
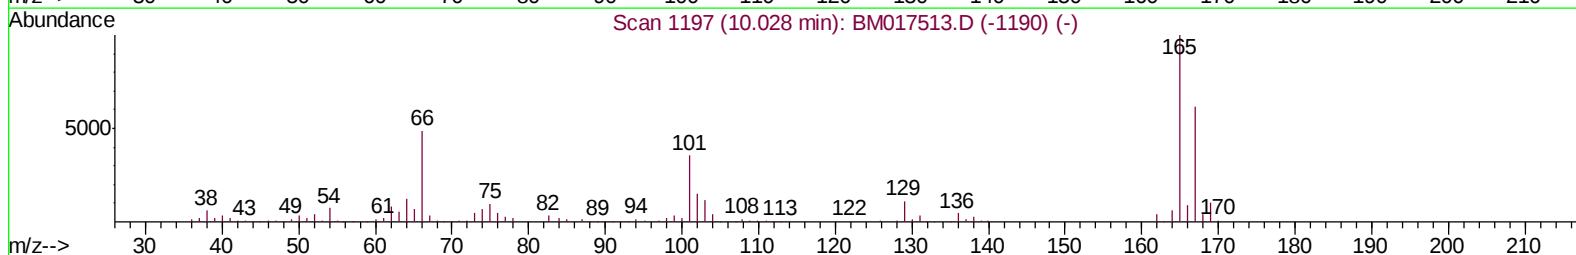
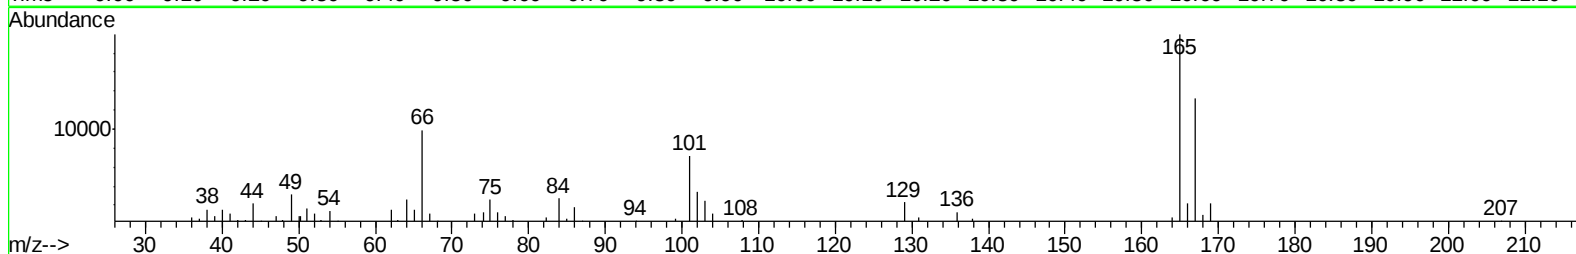


Data File : BM017515.D
Acq On : 05 Nov 2018 14:41
Operator : MJ/SJ
Sample : J5701-12DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Nov 06 00:37:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 06 00:34:52 2018
Response via : Initial Calibration

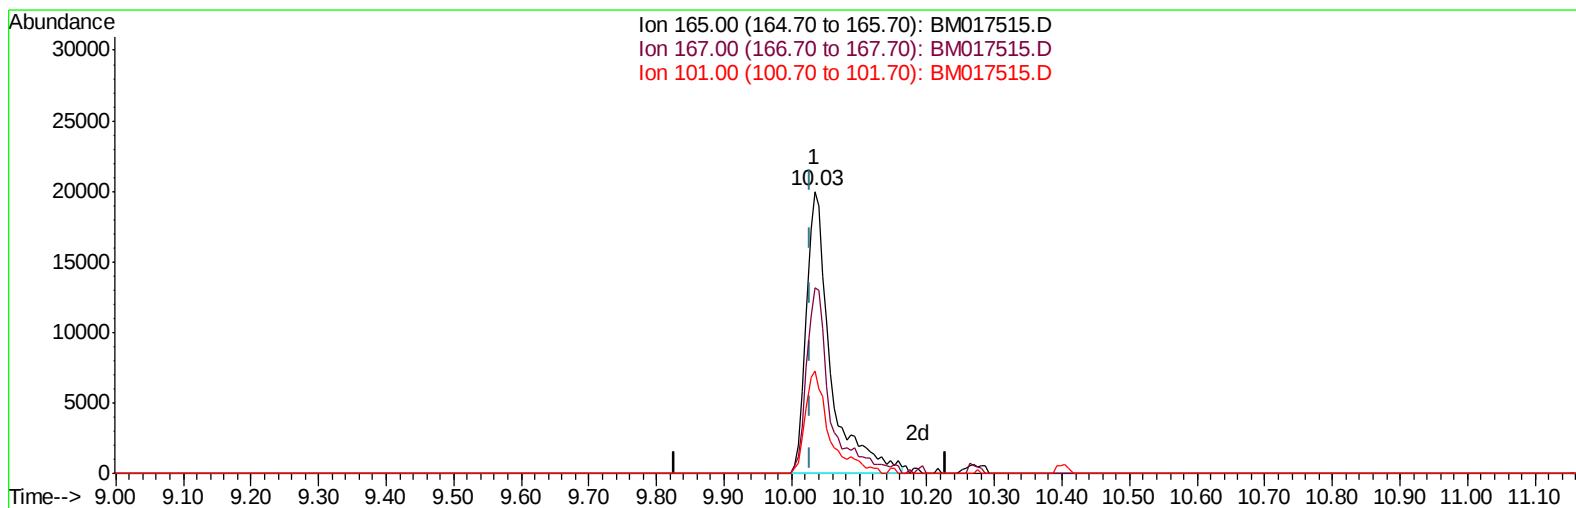

TIC: BM017515.D

(26) 2,4-Dichlorophenol-d3 (S)

10.034min (+0.006) 2.91ng/ul m

response 49688

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	65.99
101.00	34.30	36.21
0.00	0.00	0.00