
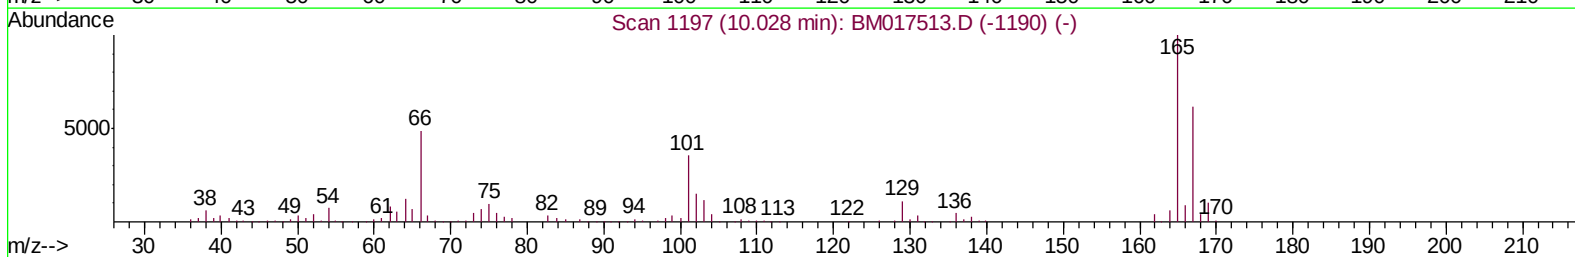
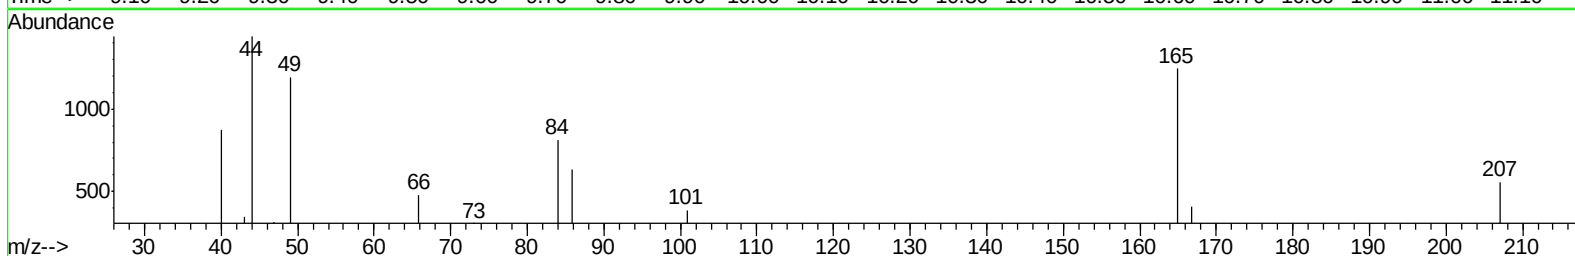


Data File : BM017516.D
Acq On : 05 Nov 2018 15:17
Operator : MJ/SJ
Sample : J5701-11DL 30X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Nov 06 00:37:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 06 00:34:52 2018
Response via : Initial Calibration

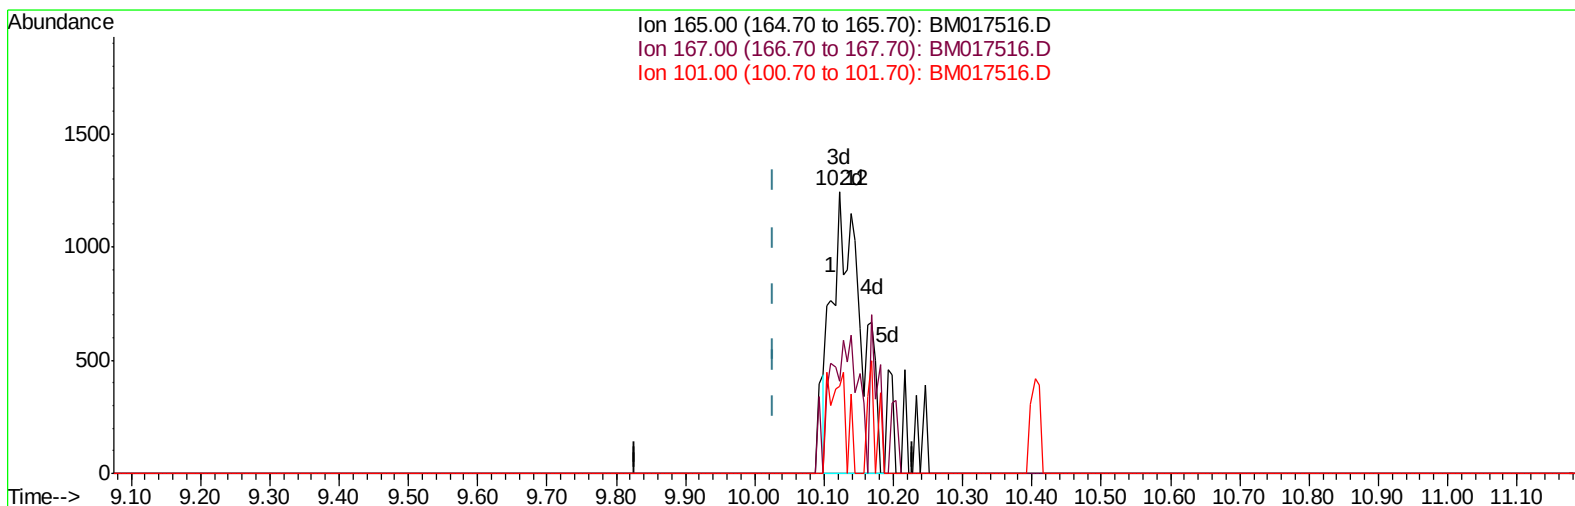

TIC: BM017516.D

(26) 2,4-Dichlorophenol-d3 (S)

10.122min (+0.094) 0.27ng/ul m

response 3614

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	32.64#
101.00	34.30	31.03
0.00	0.00	0.00