

Data File : BM017517.D

Acq On : 05 Nov 2018 15:53

Operator : MJ/SJ

Sample : SSTDCCC020

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Nov 06 00:37:52 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Nov 06 00:34:52 2018

Response via : Initial Calibration

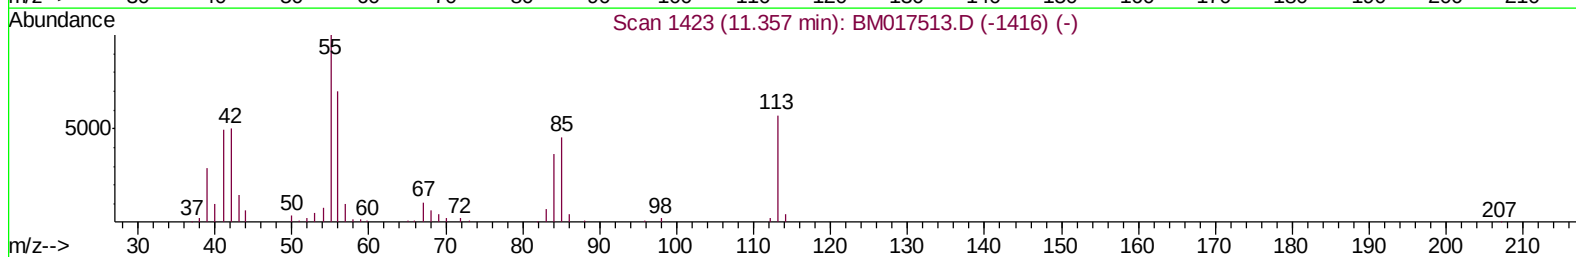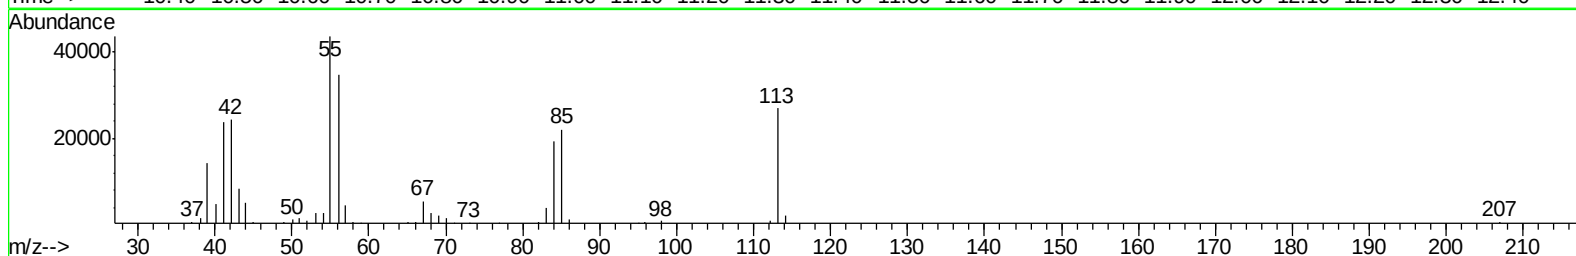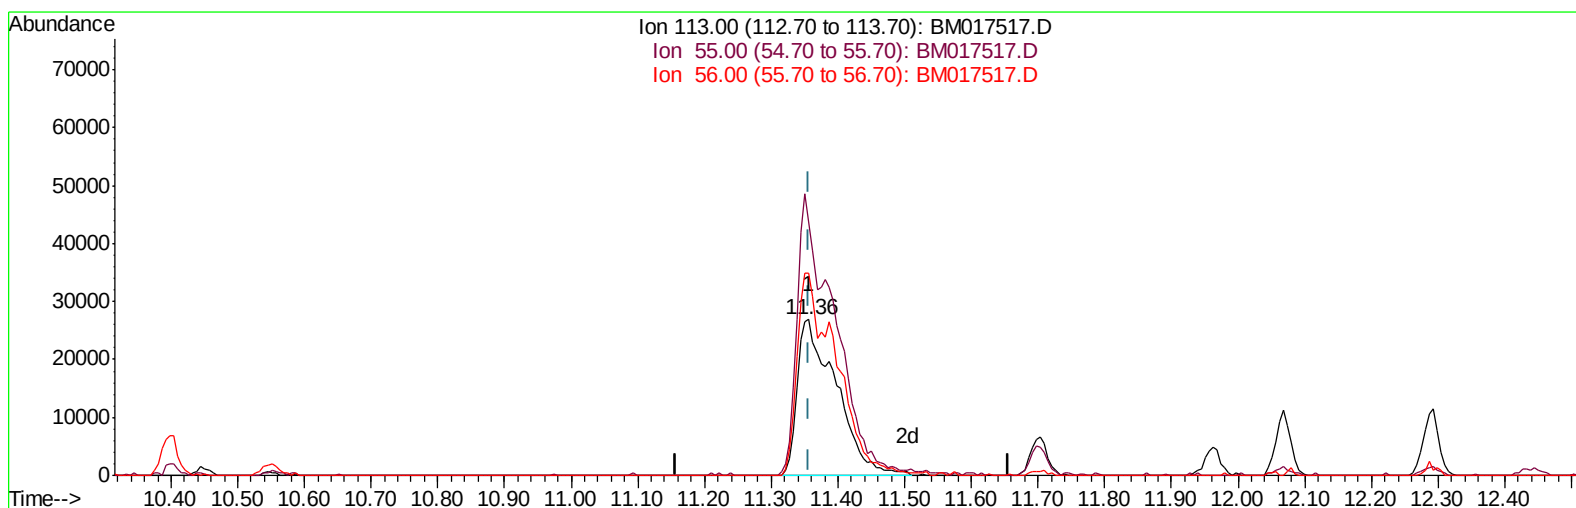

TIC: BM017517.D

(32) Caprolactam

11.357min (-0.000) 22.24ng/ul m

response 108059

Ion	Exp%	Act%
113.00	100	100
55.00	156.90	162.29
56.00	125.50	129.24
0.00	0.00	0.00