
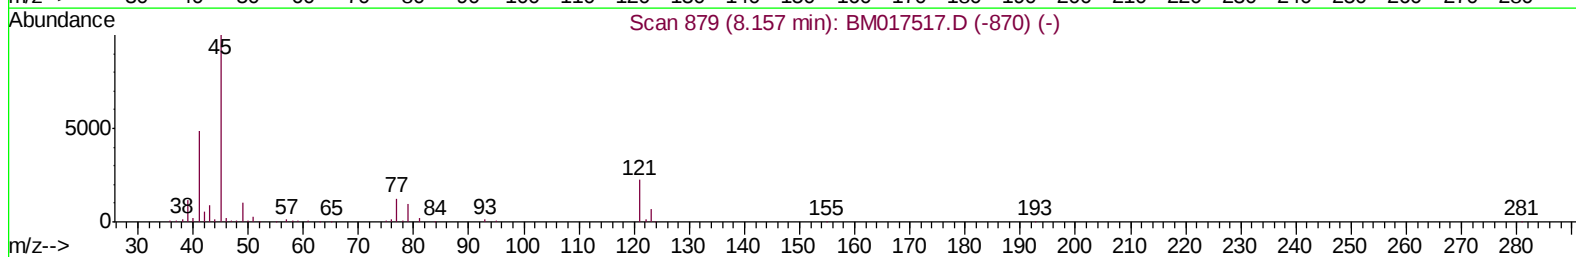
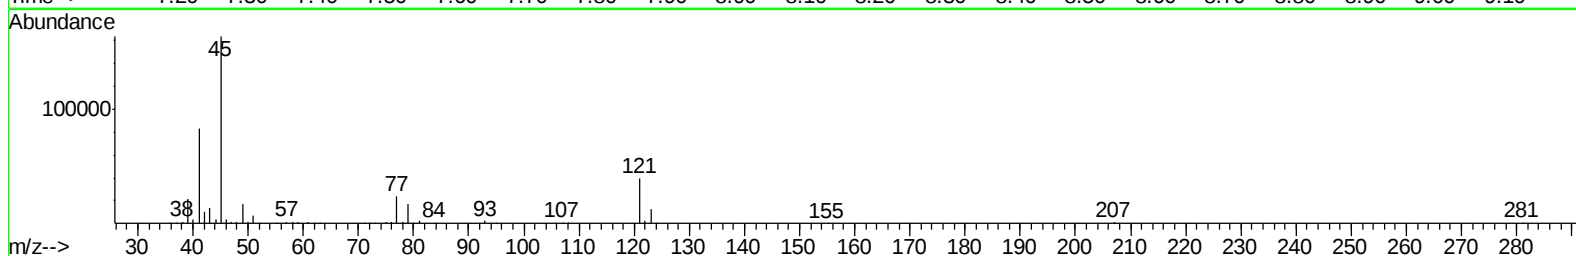


Data File : BM017520.D
Acq On : 05 Nov 2018 19:43
Operator : MJ/SJ
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Nov 06 01:25:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 06 01:23:03 2018
Response via : Initial Calibration

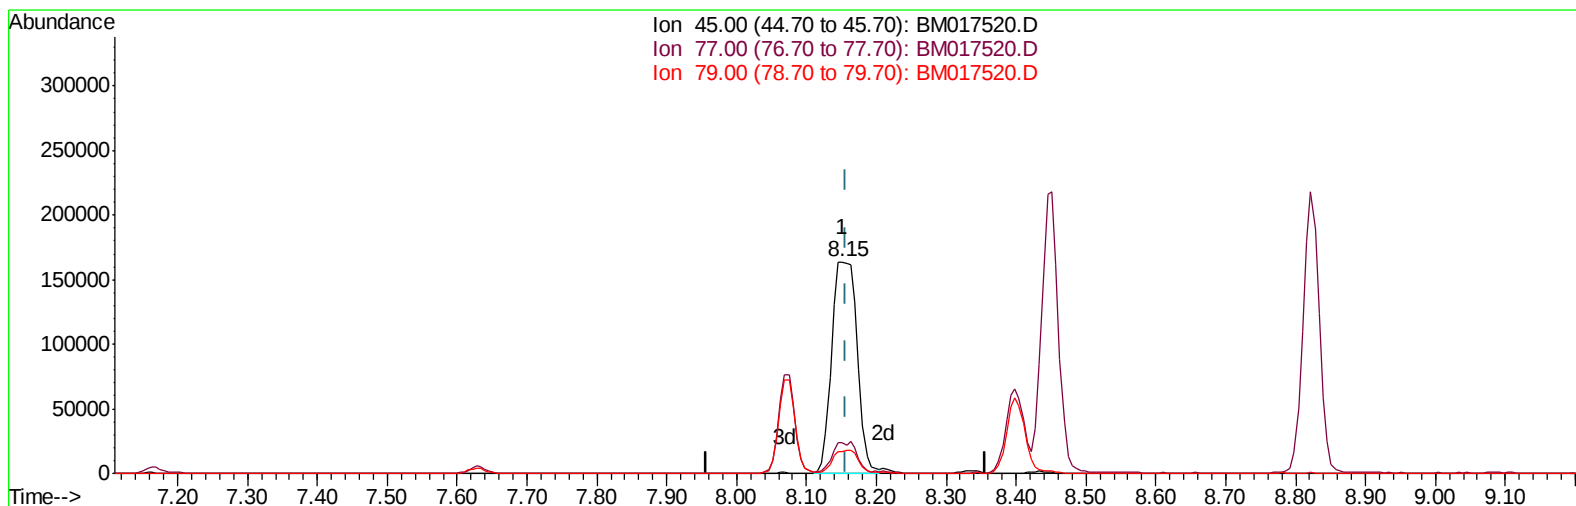

TIC: BM017520.D

(12) 2,2'-oxybis(1-Chloropropane)

8.151min (-0.006) 22.36ng/ul m

response 413958

Ion	Exp%	Act%
45.00	100	100
77.00	14.60	14.38
79.00	10.70	10.53
0.00	0.00	0.00