

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110518\
 Data File : BM017515.D
 Acq On : 05 Nov 2018 14:41
 Operator : MJ/SJ
 Sample : J5701-12DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 A40F9DL

Manual Integrations
 APPROVED

Sohil
 11/6/2018 1:20:34 PM

Quant Time: Nov 06 00:52:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 06 00:34:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	233987	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1050266	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	617868	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1643231	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1892639	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	1977519	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	3387	0.67	ng/uL	0.01
5) Phenol-d5	6.82	99	59726	2.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	45382	3.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	52419	3.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	48761	2.89	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	25127	3.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	27750	3.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	49688m	2.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	64373	4.61	ng/ul	0.01
44) Dimethylphthalate-d6	13.69	166	188660	3.56	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	221645	3.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.52	143	17286	1.75	ng/ul	0.03
58) Fluorene-d10	15.27	176	167397	3.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	18038m	1.58	ng/ul	0.00
71) Anthracene-d10	17.13	188	255764	3.14	ng/ul	0.00
79) Pyrene-d10	19.43	212	330638	3.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	366657	3.51	ng/ul	0.00

Target Compounds					Qvalue	
84) Bis(2-ethylhexyl)phthalate	21.15	149	3320982	51.797	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110518\
Data File : BM017515.D
Acq On : 05 Nov 2018 14:41
Operator : MJ/SJ
Sample : J5701-12DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A40F9DL

Quant Time: Nov 06 00:52:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 06 00:34:52 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
11/6/2018 1:20:34 PM

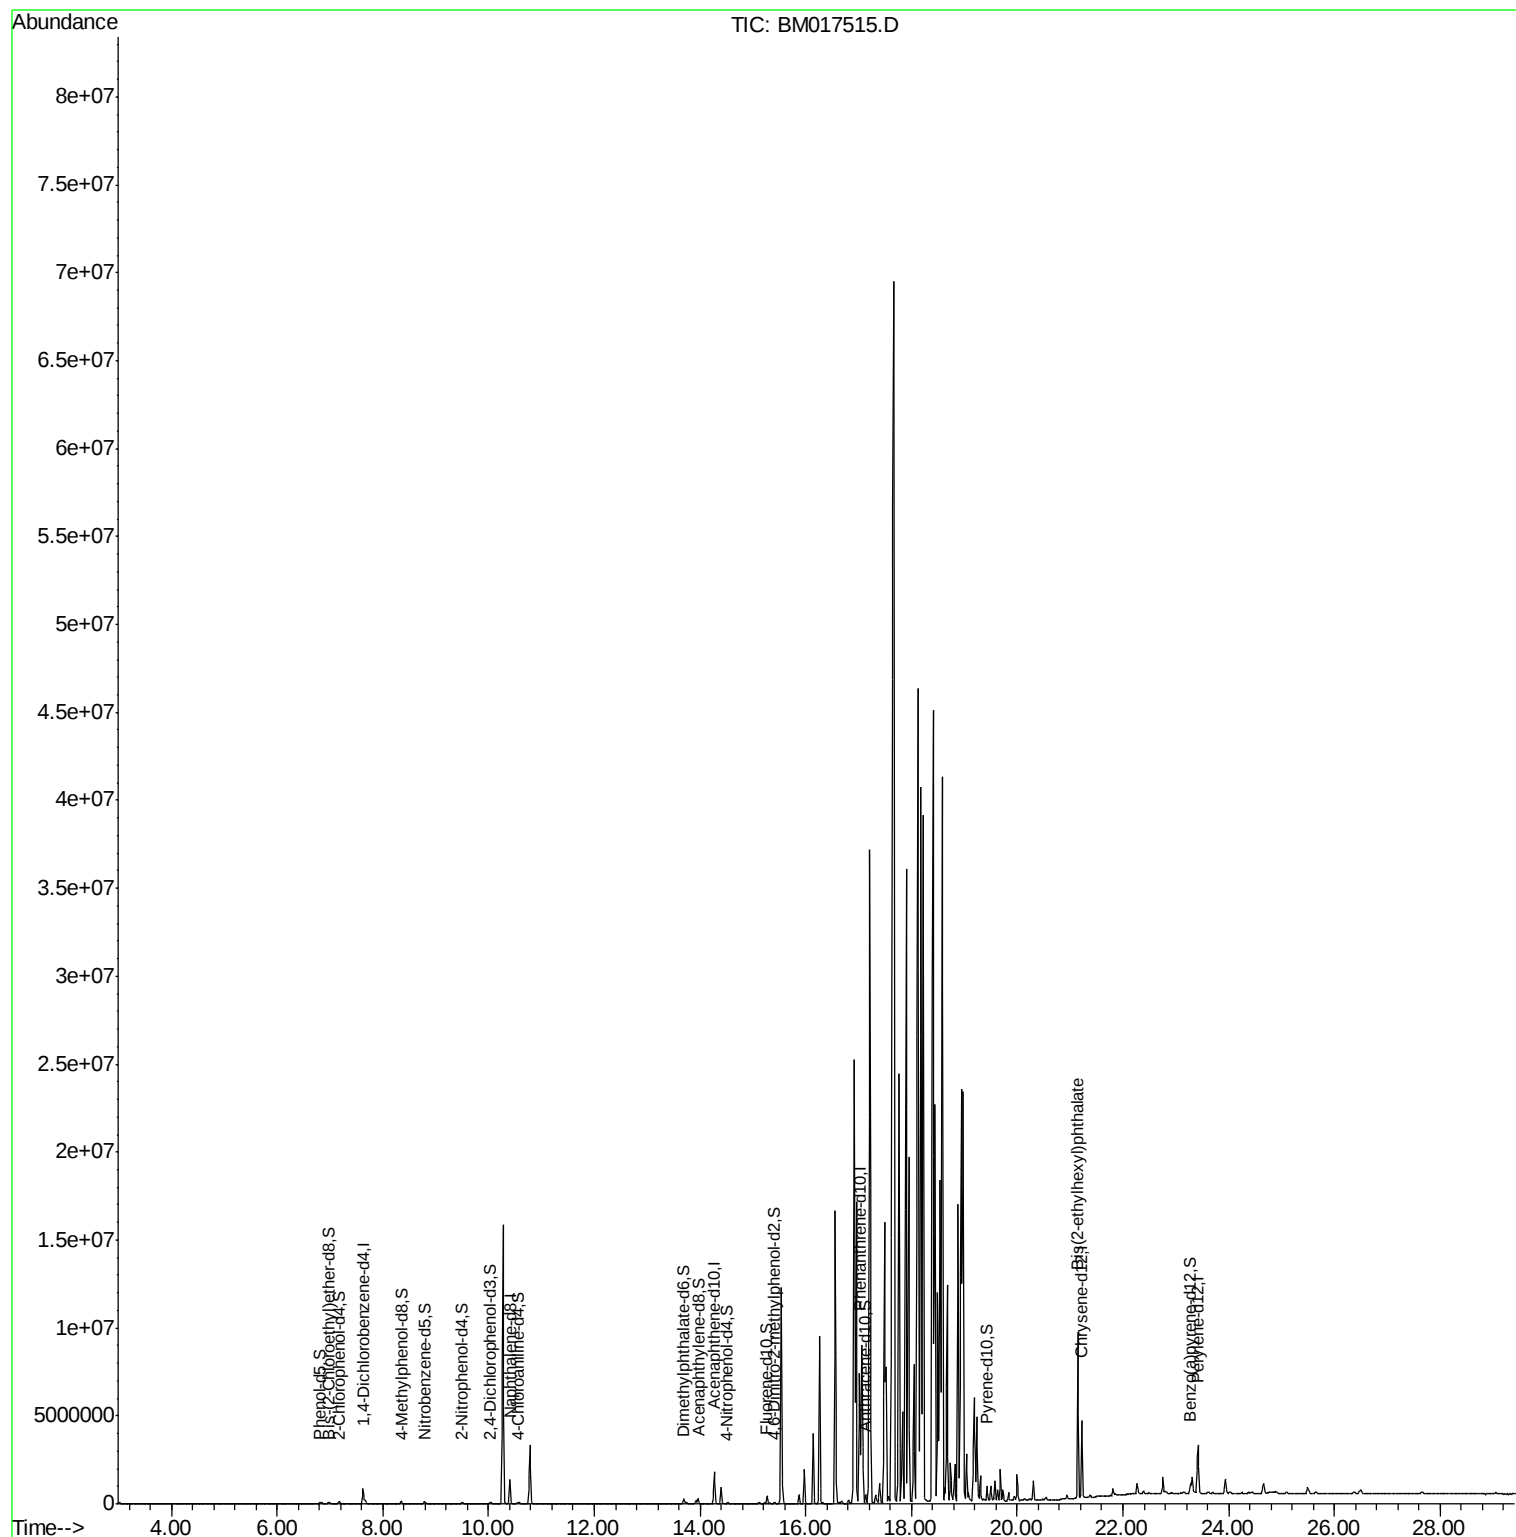

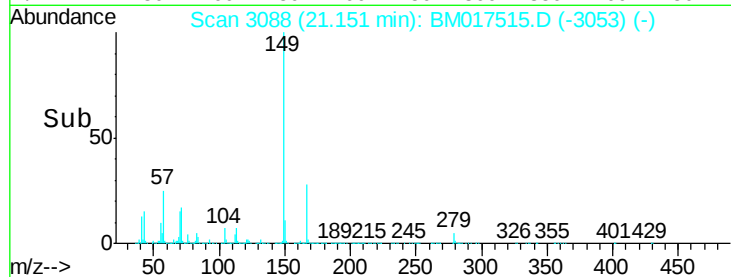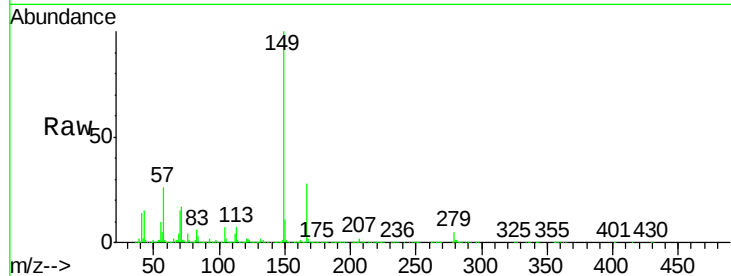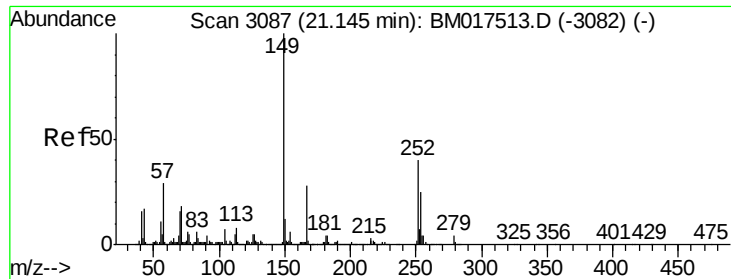

#84

Bis(2-ethylhexyl)phthalate

Concen: 51.797 ng/ul

RT: 21.15 min Scan# 3088

Delta R.T. 0.01 min

Lab File: BM017515.D

Acq: 05 Nov 2018 14:41

Instrument :

BNA_M

ClientSampleId :

A40F9DL

Tgt Ion:149 Resp: 3320982

Ion Ratio Lower Upper

149 100

167 28.3 23.0 34.6

279 4.9 4.1 6.1

Manual Integrations

APPROVED

Sohil

11/6/2018 1:20:34 PM

