

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110519\
 Data File : BM023603.D
 Acq On : 05 Nov 2019 12:25
 Operator : JU
 Sample : K5567-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNBS

Quant Time: Nov 06 05:50:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 05:47:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	380984	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	1571913	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.25	164	954472	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	2045994	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2031784	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2418131	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	42269	5.27	ng/uL	0.00
5) Phenol-d5	6.78	99	215366	6.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	497245	26.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	556803	22.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	362976	13.97	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	326282	27.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	338516	25.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	582266	22.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	56500	1.90	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	2059671	28.42	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	2377952	28.64	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	45010	3.58	ng/ul	0.00
58) Fluorene-d10	15.24	176	1770759	28.85	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	234402	18.40	ng/ul	0.00
71) Anthracene-d10	17.10	188	2955841	30.57	ng/ul	0.00
79) Pyrene-d10	19.40	212	3296565	29.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	3928097	31.89	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.72	163	311688	4.283	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110519\
Data File : BM023603.D
Acq On : 05 Nov 2019 12:25
Operator : JU
Sample : K5567-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNB8

Quant Time: Nov 06 05:50:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 05:47:35 2019
Response via : Initial Calibration

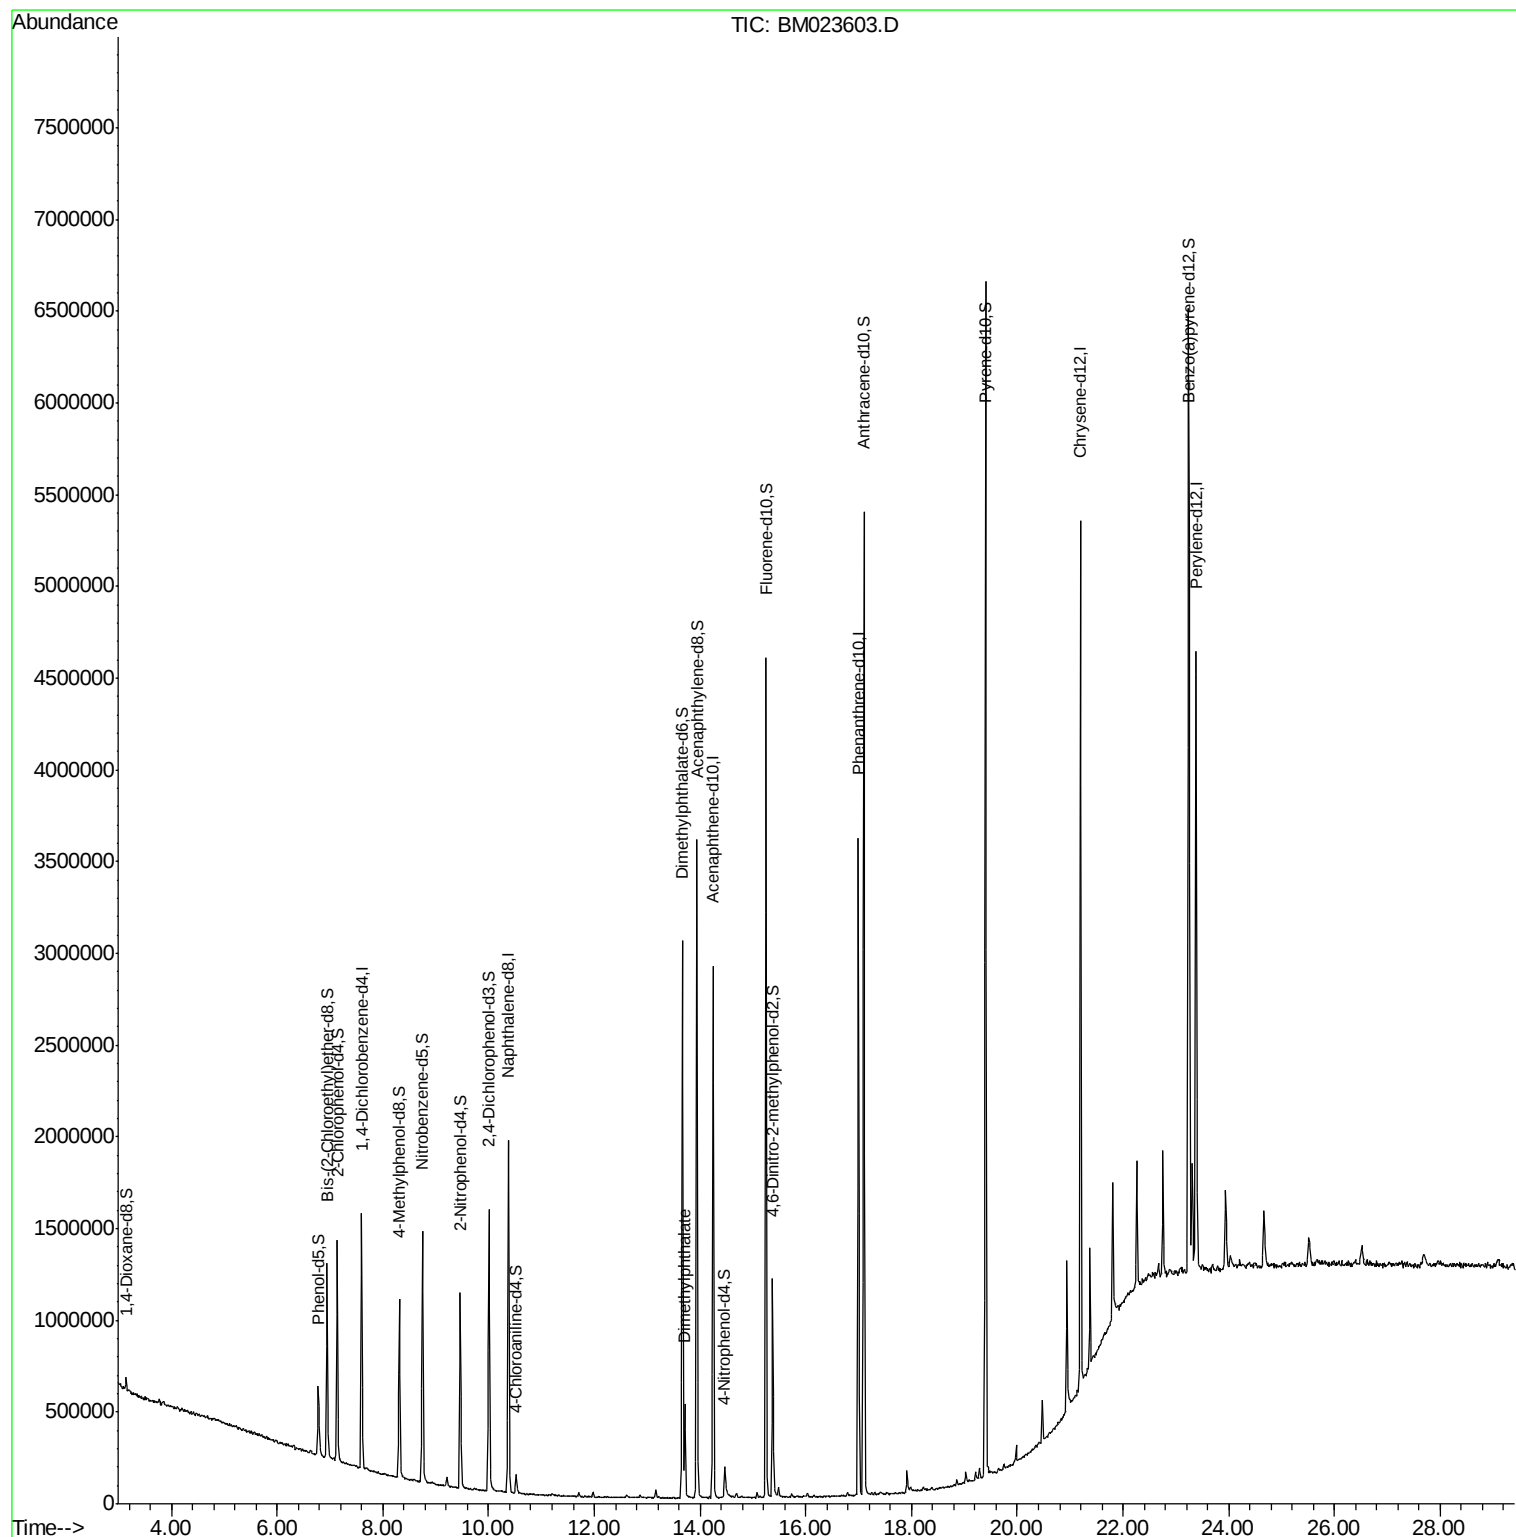

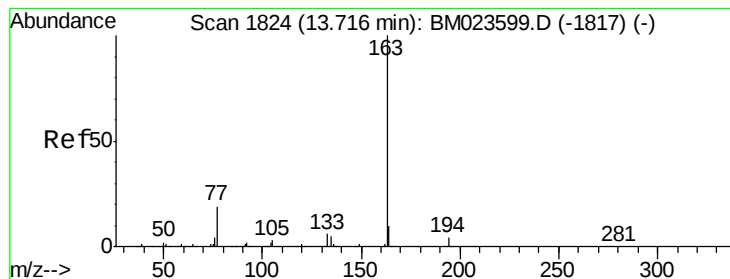

#45

Dimethylphthalate

Concen: 4.283 ng/ul

RT: 13.72 min Scan# 1824

Delta R.T. -0.00 min

Lab File: BM023603.D

Acq: 05 Nov 2019 12:25

Instrument :

BNA_M

ClientSampleId :

JLNB8



Tot Ion:163 Resp: 311688

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.4 7.9 11.9

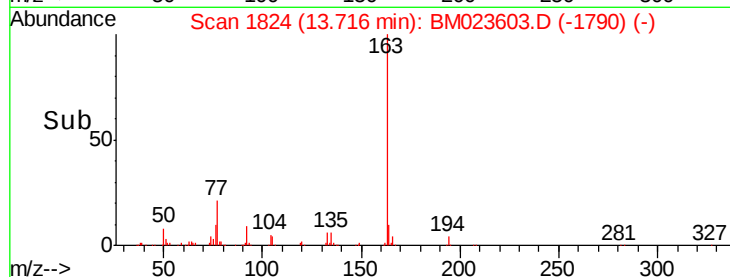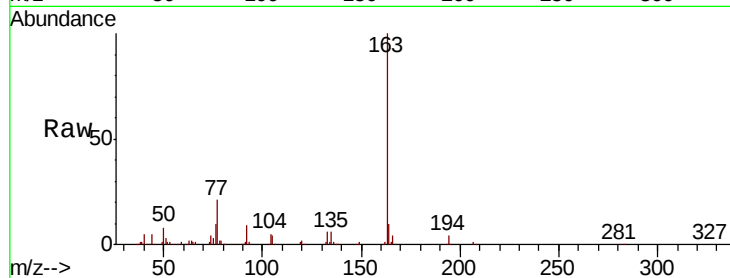

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

