

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110519\
 Data File : BM023604.D
 Acq On : 05 Nov 2019 13:00
 Operator : JU
 Sample : K5567-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLN9

Quant Time: Nov 06 05:50:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 05:47:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	391794	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	1631378	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.25	164	1001451	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	2116716	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2067098	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2527670	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	47054	5.70	ng/uL	0.00
5) Phenol-d5	6.78	99	187649	5.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	450399	23.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	504713	19.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	328724	12.30	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	299647	24.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	308325	22.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	530132	19.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	61497	2.00	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	1966857	25.86	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	2253132	25.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	45485	3.45	ng/ul	0.00
58) Fluorene-d10	15.24	176	1733545	26.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	228015	17.30	ng/ul	0.00
71) Anthracene-d10	17.10	188	2988307	29.87	ng/ul	0.00
79) Pyrene-d10	19.40	212	3318274	29.19	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	3948413	30.66	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.72	163	205879	2.696 ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110519\
Data File : BM023604.D
Acq On : 05 Nov 2019 13:00
Operator : JU
Sample : K5567-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNB9

Quant Time: Nov 06 05:50:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 05:47:35 2019
Response via : Initial Calibration

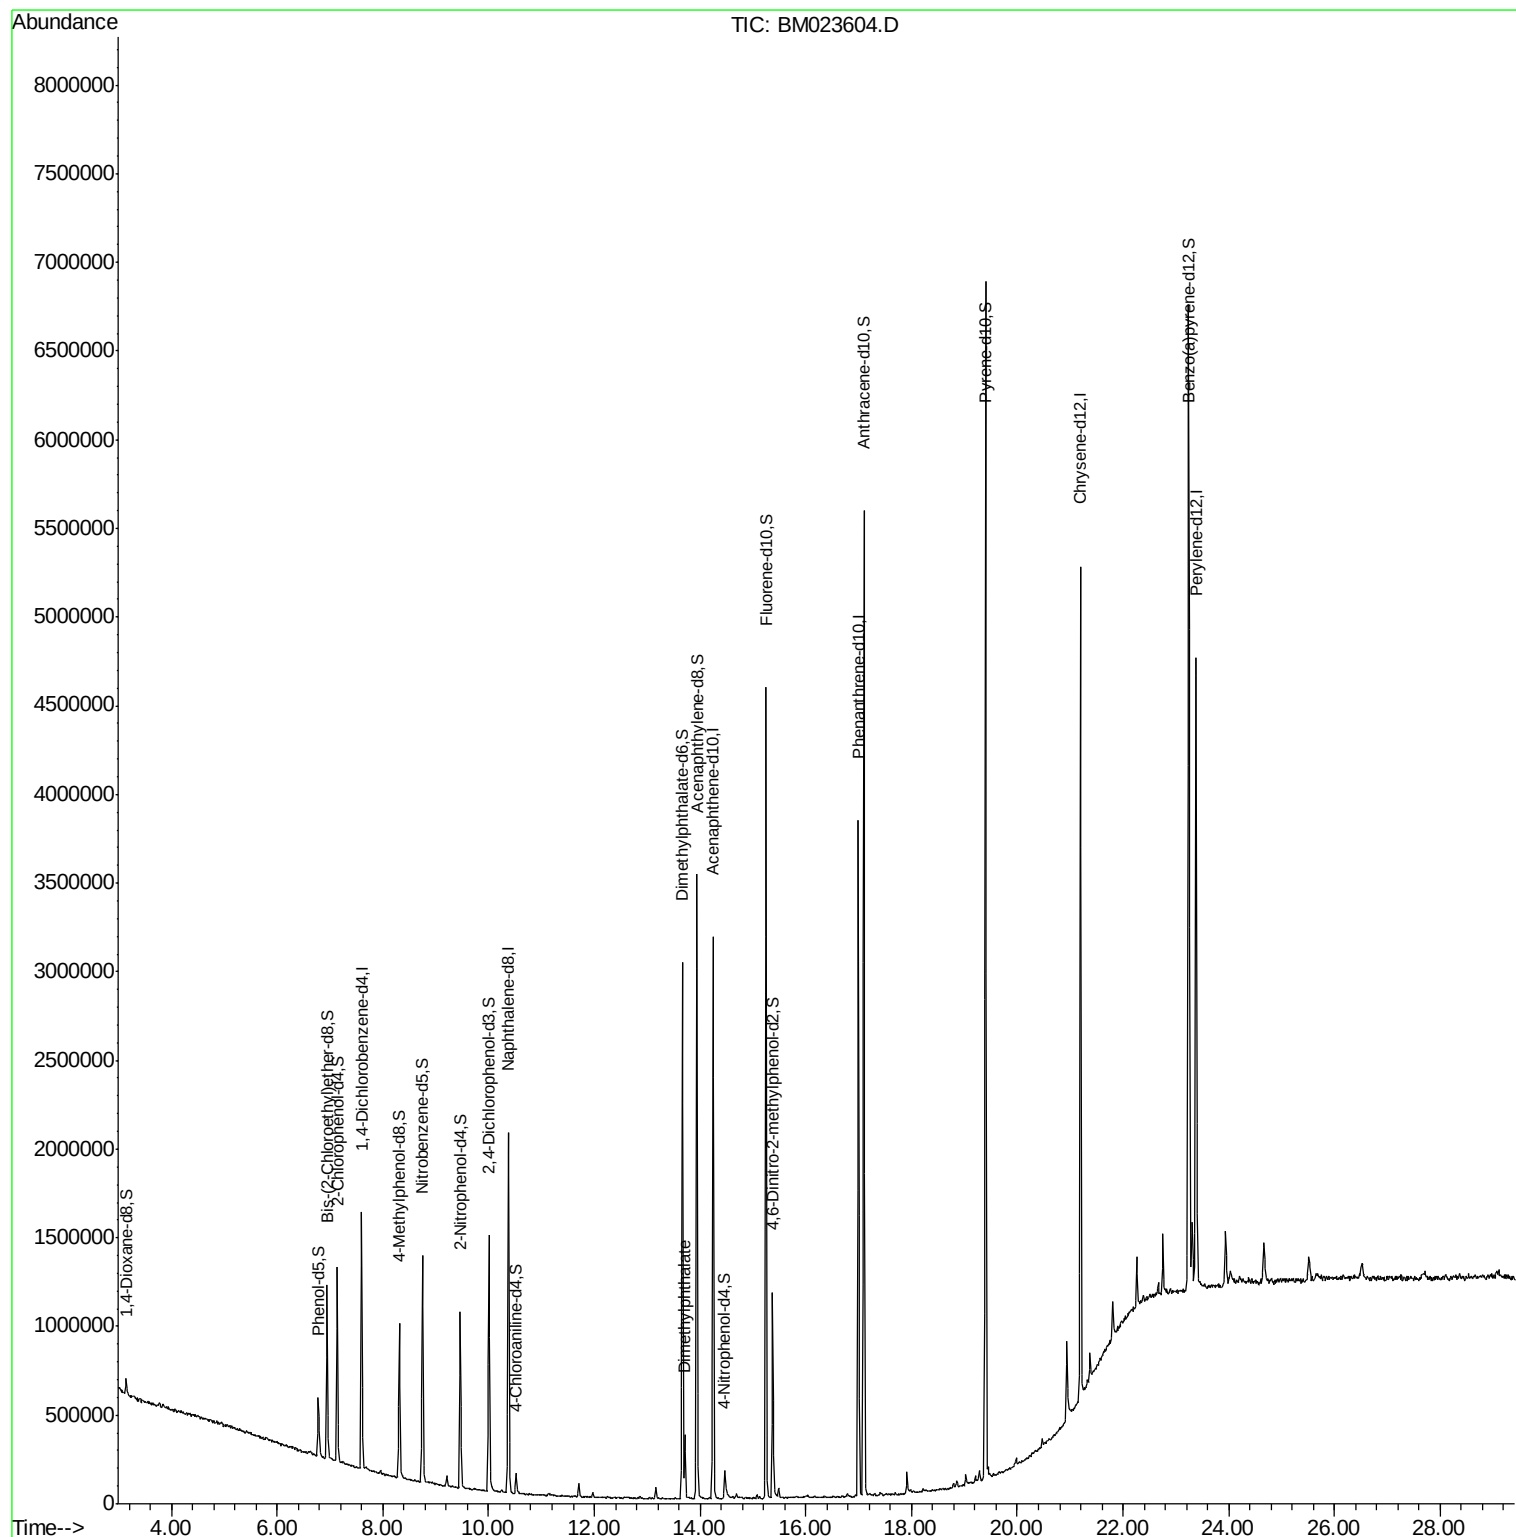

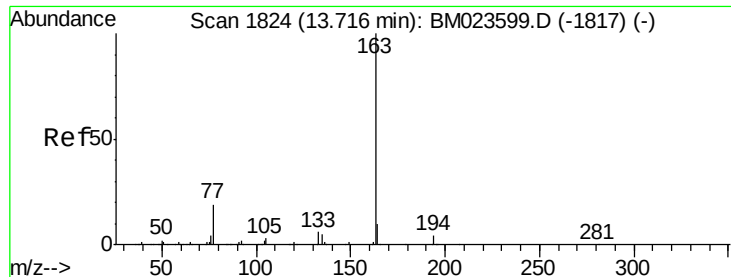

#45

Dimethylphthalate

Concen: 2.696 ng/ul

RT: 13.72 min Scan# 1824

Delta R.T. -0.00 min

Lab File: BM023604.D

Acq: 05 Nov 2019 13:00

Instrument :

BNA_M

ClientSampleId :

JLNB9

Tot Ion:163 Resp: 205879

Ion Ratio Lower Upper

163 100

194 4.3 3.3 4.9

164 11.1 7.9 11.9

