

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110519\
 Data File : BM023605.D
 Acq On : 05 Nov 2019 13:36
 Operator : JU
 Sample : K5567-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNC3

Quant Time: Nov 06 05:50:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 05:47:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	393873	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	1588808	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.25	164	933760	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	2013618	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	2026252	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	2512459	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	41558	5.01	ng/uL	0.00
5) Phenol-d5	6.78	99	178561	5.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	485038	25.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	514109	19.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	311464	11.59	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	310930	26.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	319093	24.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	531541	20.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	58781	1.96	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	1831181	25.82	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	2177517	26.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	34848	2.84	ng/ul	0.00
58) Fluorene-d10	15.24	176	1679006	27.96	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	220639	17.60	ng/ul	0.00
71) Anthracene-d10	17.10	188	2935110	30.84	ng/ul	0.00
79) Pyrene-d10	19.40	212	3340496	29.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	4033018	31.51	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.72	163	89498	1.257	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110519\
Data File : BM023605.D
Acq On : 05 Nov 2019 13:36
Operator : JU
Sample : K5567-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNC3

Quant Time: Nov 06 05:50:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 05:47:35 2019
Response via : Initial Calibration

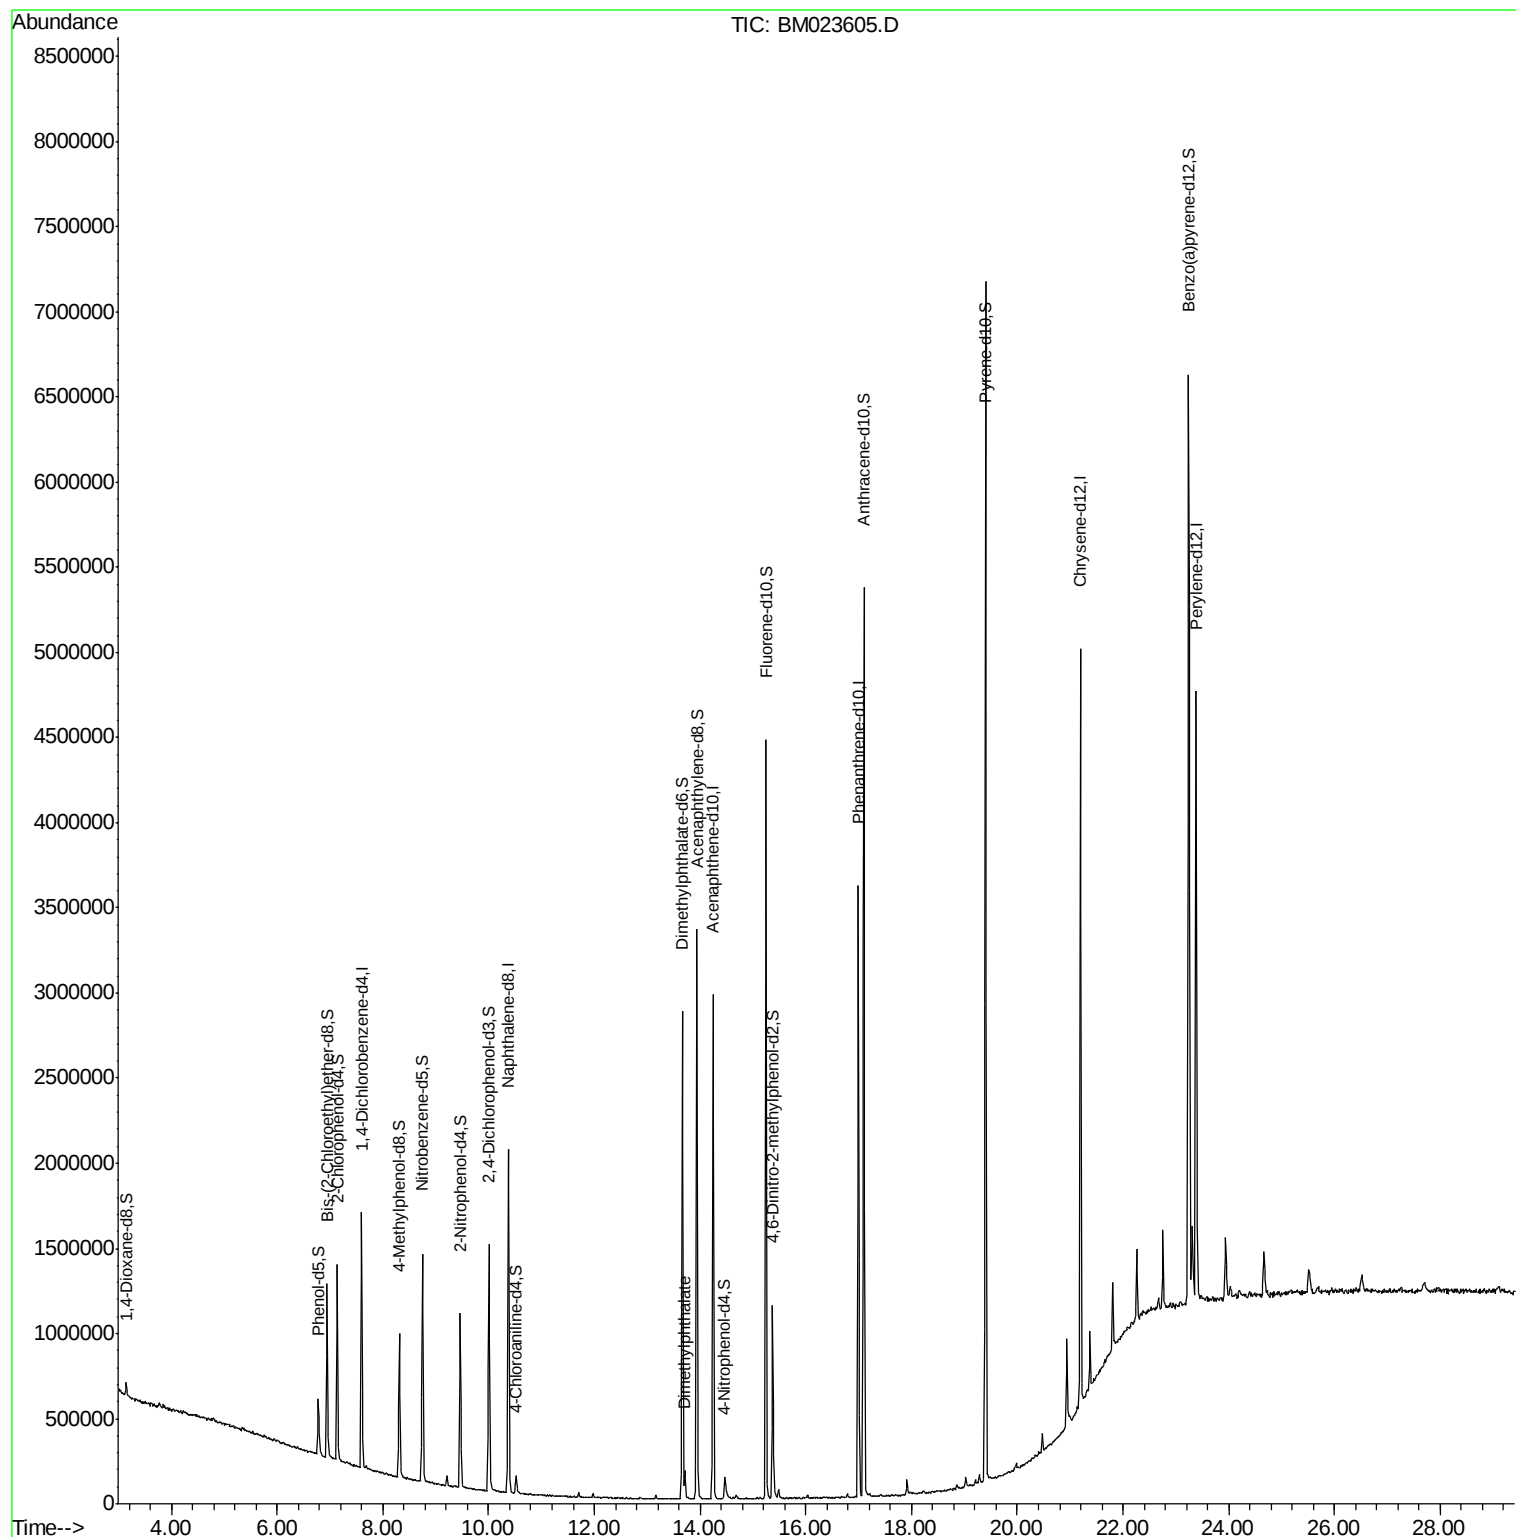

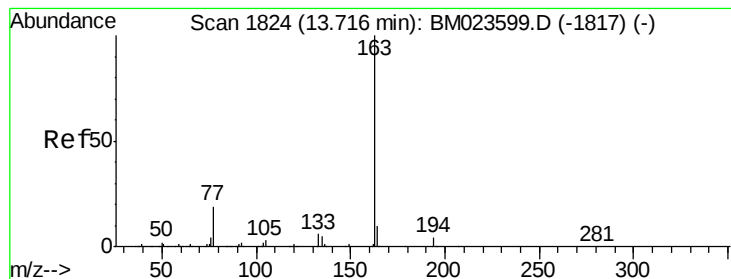

#45

Dimethylphthalate

Concen: 1.257 ng/ul

RT: 13.72 min Scan# 1824

Delta R.T. -0.00 min

Lab File: BM023605.D

Acq: 05 Nov 2019 13:36

Instrument :

BNA_M

ClientSampleId :

JLNC3


Tot Ion:163 Resp: 89498

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 9.9 7.9 11.9

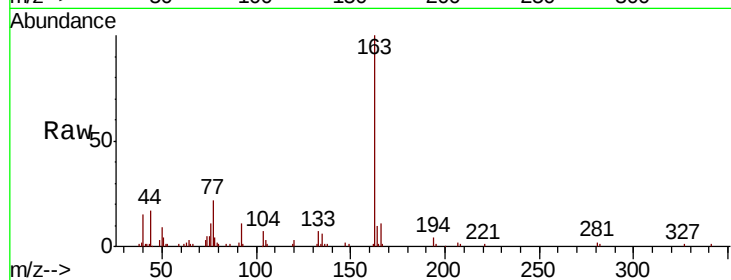

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

