

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110519\
 Data File : BM023613.D
 Acq On : 05 Nov 2019 18:23
 Operator : JU
 Sample : K5567-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLNE0

Quant Time: Nov 06 07:23:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 06 07:21:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	422451	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	1746221	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.25	164	1050738	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.00	188	2271104	20.00	ng/ul	0.00
78) Chrysene-d12	21.19	240	2252456	20.00	ng/ul	0.00
86) Perylene-d12	23.38	264	2778276	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	44305	4.98	ng/uL	0.00
5) Phenol-d5	6.78	99	234056	6.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	522857	25.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	583267	21.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	385886	13.39	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	336922	25.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	342083	23.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	609424	21.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	54006	1.64	ng/ul	0.00
44) Dimethylphthalate-d6	13.67	166	2061022	25.83	ng/ul	0.00
47) Acenaphthylene-d8	13.94	160	2469898	27.02	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	44720	3.24	ng/ul	0.00
58) Fluorene-d10	15.25	176	1830036	27.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.37	200	205944	14.57	ng/ul	0.00
71) Anthracene-d10	17.10	188	3014243	28.08	ng/ul	0.00
79) Pyrene-d10	19.40	212	3422163	27.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.24	264	4082282	28.84	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.72	163	94031	1.174 ng/ul# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM110519\
Data File : BM023613.D
Acq On : 05 Nov 2019 18:23
Operator : JU
Sample : K5567-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLNE0

Quant Time: Nov 06 07:23:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 06 07:21:06 2019
Response via : Initial Calibration

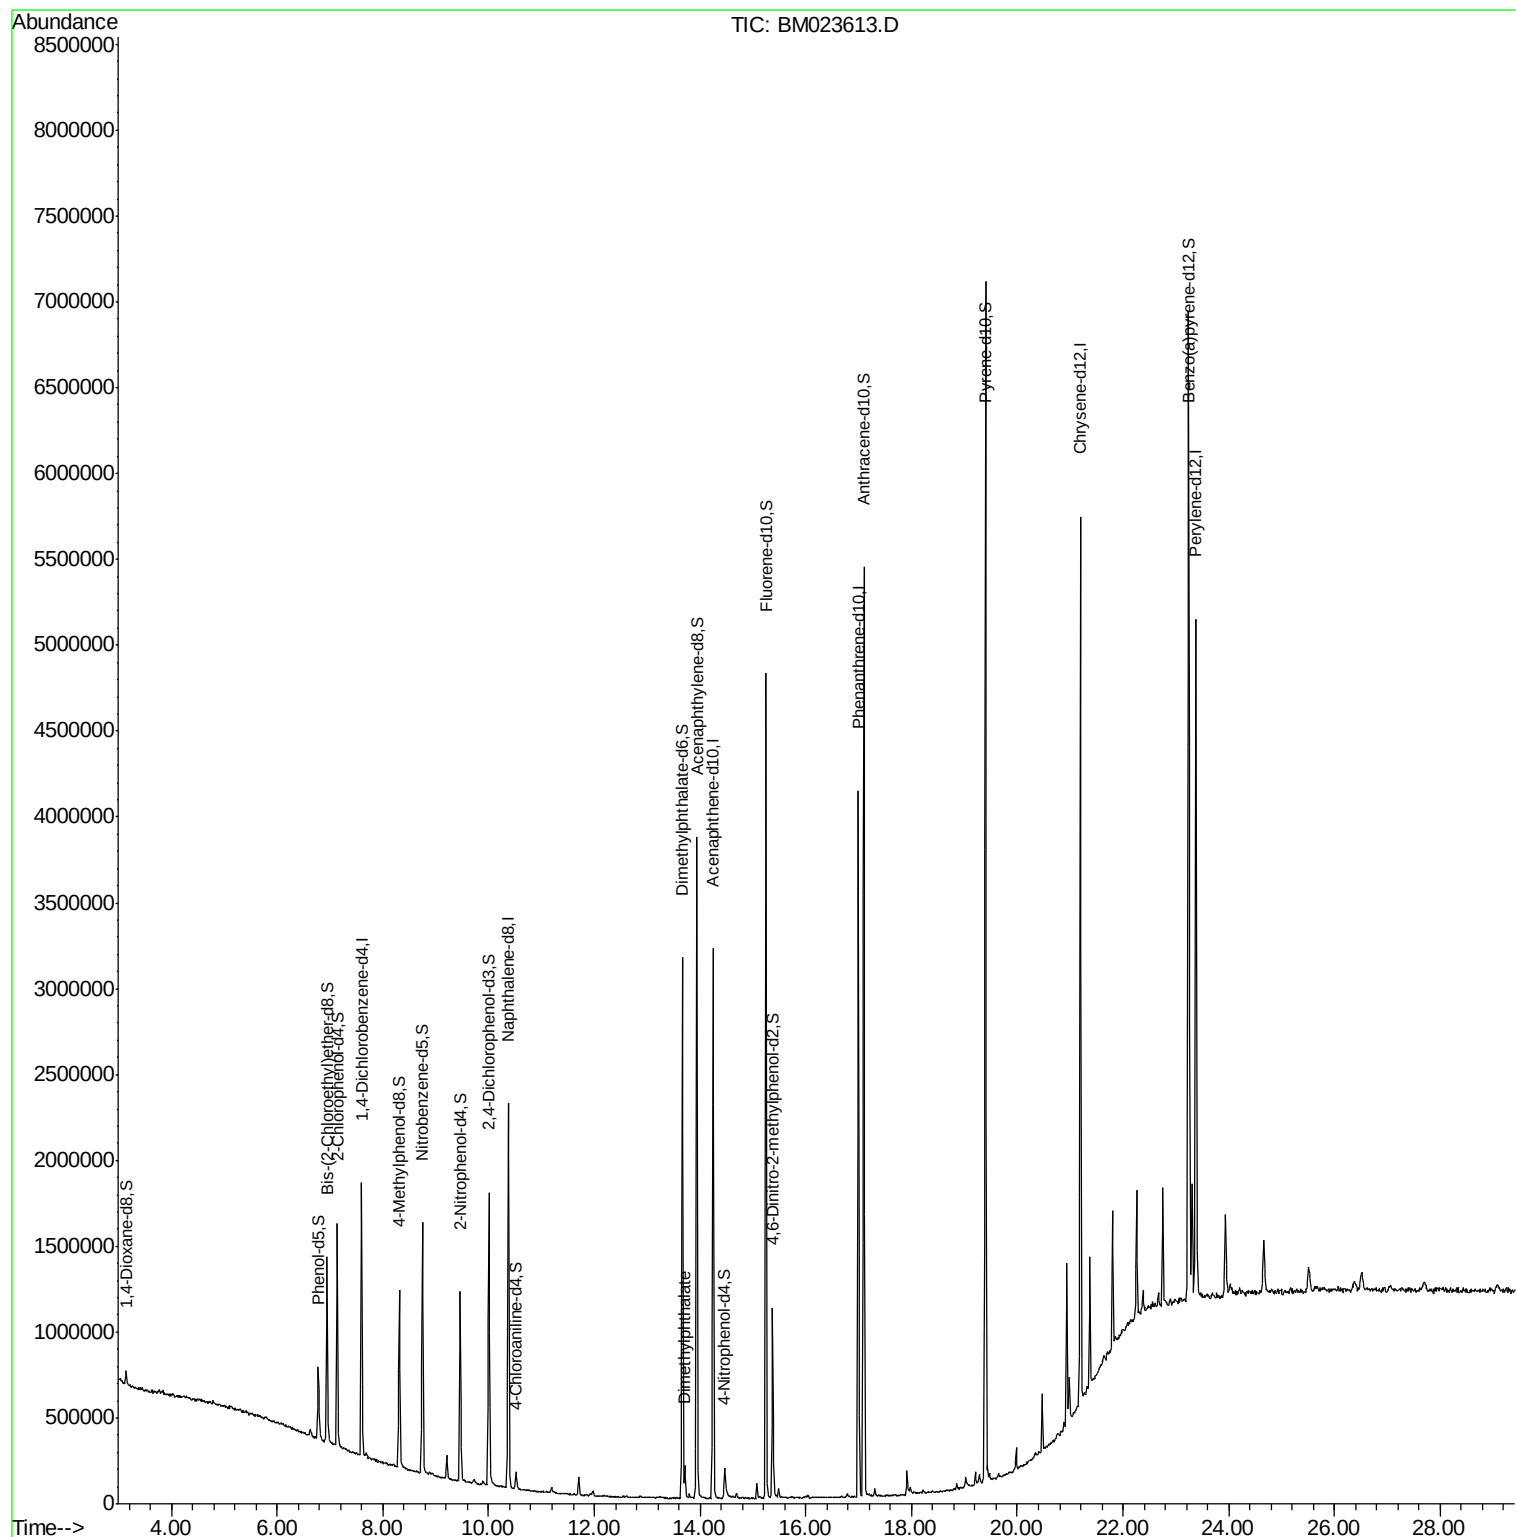

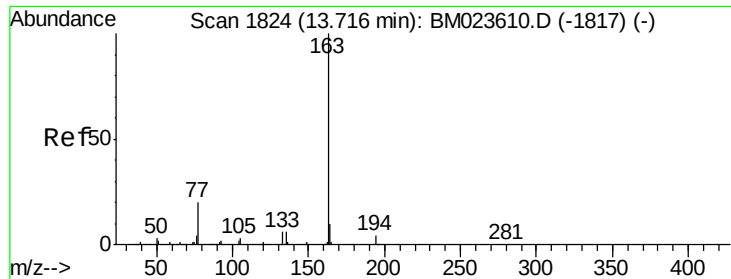

#45

Dimethylphthalate

Concen: 1.174 ng/ul

RT: 13.72 min Scan# 1824

Delta R.T. 0.00 min

Lab File: BM023613.D

Acq: 05 Nov 2019 18:23

Instrument :

BNA_M

ClientSampleId :

JLNE0

Tot Ion:163 Resp: 94031

Ion Ratio Lower Upper

163 100

194 5.1 3.3 4.9#

164 9.6 7.9 11.9

