

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110618\
 Data File : BM017526.D
 Acq On : 06 Nov 2018 13:32
 Operator : MJ/SJ
 Sample : J5704-03MEDL 100X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40F8MEDL

Manual Integrations
 APPROVED

Sohil
 11/6/2018 4:36:54 PM

Quant Time: Nov 06 14:07:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 06 12:04:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	188402	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	793574	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	498368	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1227478	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1527913	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	1643828	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	302	0.07	ng/uL	0.00
5) Phenol-d5	6.85	99	618	0.04	ng/ul	0.04
7) Bis-(2-Chloroethyl)ether-d	6.99	67	1569	0.16	ng/ul	0.01
9) 2-Chlorophenol-d4	7.17	132	1756	0.13	ng/ul	0.01
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.66	131	114	0.01	ng/ul	0.11
44) Dimethylphthalate-d6	13.72	166	9713	0.23	ng/ul	0.03
47) Acenaphthylene-d8	13.97	160	11060	0.21	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.28	176	11204	0.30	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	17.14	188	21970m	0.36	ng/ul	0.02
79) Pyrene-d10	19.44	212	17682	0.25	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.28	264	21328	0.25	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
84) Bis(2-ethylhexyl)phthalate	21.14	149	1691637	32.682	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110618\
Data File : BM017526.D
Acq On : 06 Nov 2018 13:32
Operator : MJ/SJ
Sample : J5704-03MEDL 100X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A40F8MEDL

Manual Integrations
APPROVED

Sohil
11/6/2018 4:36:54 PM

Quant Time: Nov 06 14:07:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 06 12:04:23 2018
Response via : Initial Calibration

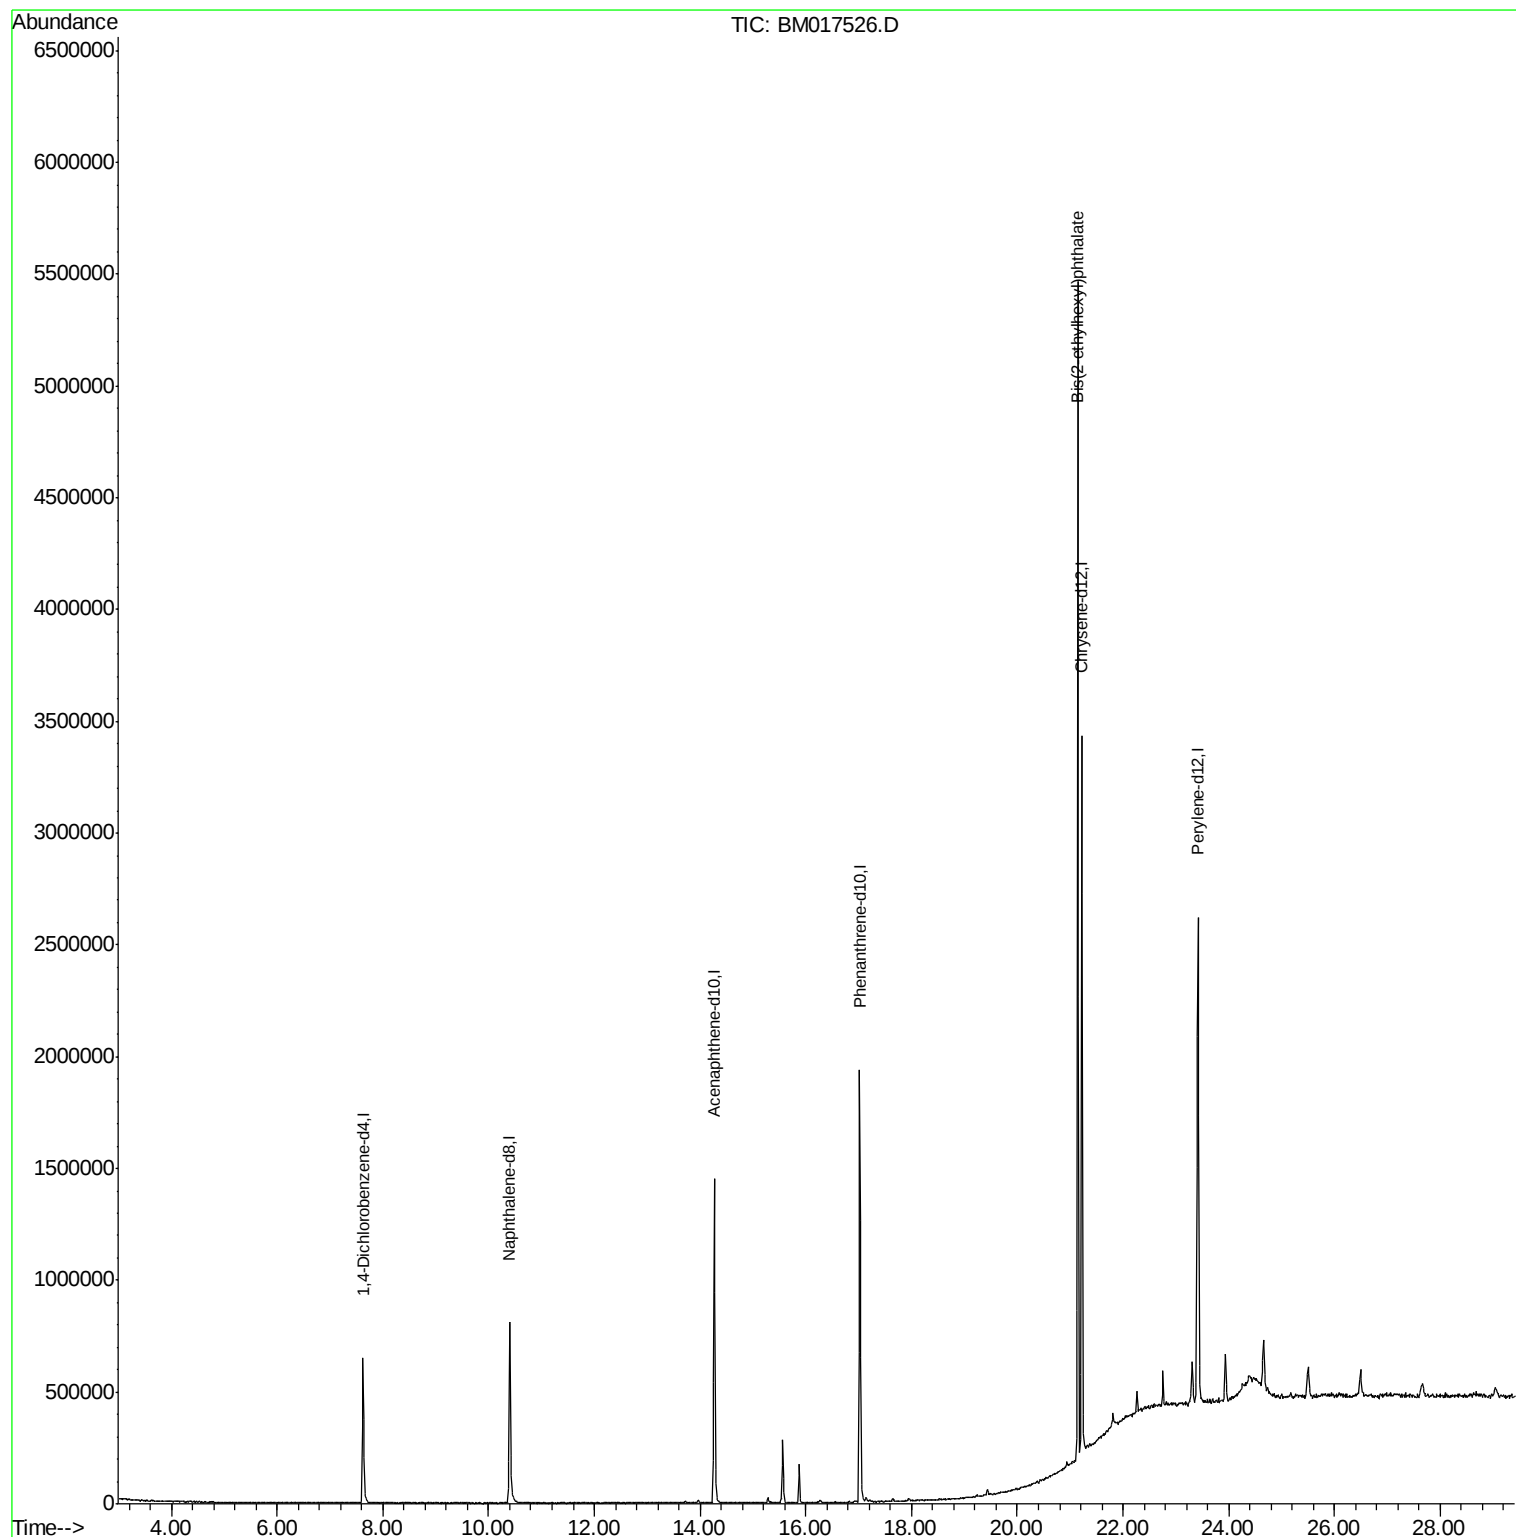

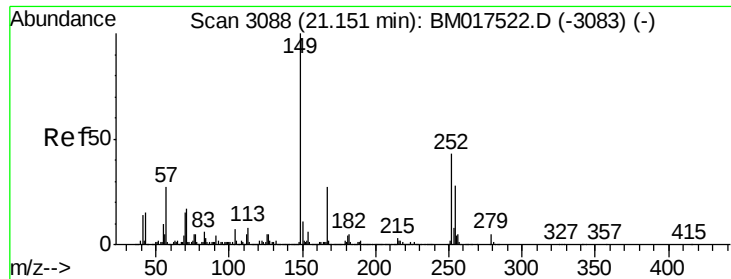

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 32.682 ng/ul
 RT: 21.14 min Scan# 3087
 Delta R.T. -0.01 min
 Lab File: BM017526.D
 Acq: 06 Nov 2018 13:32

Instrument :
 BNA_M
 ClientSampleId :
 A40F8MEDL

Tgt Ion	Ratio	Lower	Upper
149	100		
167	27.1	23.0	34.6
279	4.1	4.1	6.1

Manual Integrations
 APPROVED

Sohil
 11/6/2018 4:36:54 PM

