

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110618\
 Data File : BM017529.D
 Acq On : 06 Nov 2018 15:22
 Operator : MJ/SJ
 Sample : J5704-14MEDL 200X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A40E4MEDL

Manual Integrations
 APPROVED

Sohil
 11/6/2018 4:36:56 PM

Quant Time: Nov 06 15:59:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 06 12:04:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	201895	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	855792	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	528139	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1307755	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1515118	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	1528993	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.90	99	1168	0.06	ng/ul	0.09
7) Bis-(2-Chloroethyl)ether-d	6.99	67	1064	0.10	ng/ul	0.02
9) 2-Chlorophenol-d4	7.17	132	907	0.06	ng/ul	0.01
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	10.19	165	309	0.02	ng/ul	0.16
29) 4-Chloroaniline-d4	10.67	131	341	0.03	ng/ul	0.12
44) Dimethylphthalate-d6	13.73	166	7396	0.16	ng/ul	0.03
47) Acenaphthylene-d8	13.97	160	8133	0.15	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.29	176	9977	0.25	ng/ul	0.02
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	17.14	188	21276m	0.33	ng/ul	0.02
79) Pyrene-d10	19.44	212	13970	0.20	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.28	264	13760	0.17	ng/ul	0.00

Target Compounds					Qvalue	
84) Bis(2-ethylhexyl)phthalate	21.14	149	1529165	29.793	ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110618\
Data File : BM017529.D
Acq On : 06 Nov 2018 15:22
Operator : MJ/SJ
Sample : J5704-14MEDL 200X
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A40E4MEDL

Manual Integrations
APPROVED

Sohil
11/6/2018 4:36:56 PM

Quant Time: Nov 06 15:59:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 06 12:04:23 2018
Response via : Initial Calibration

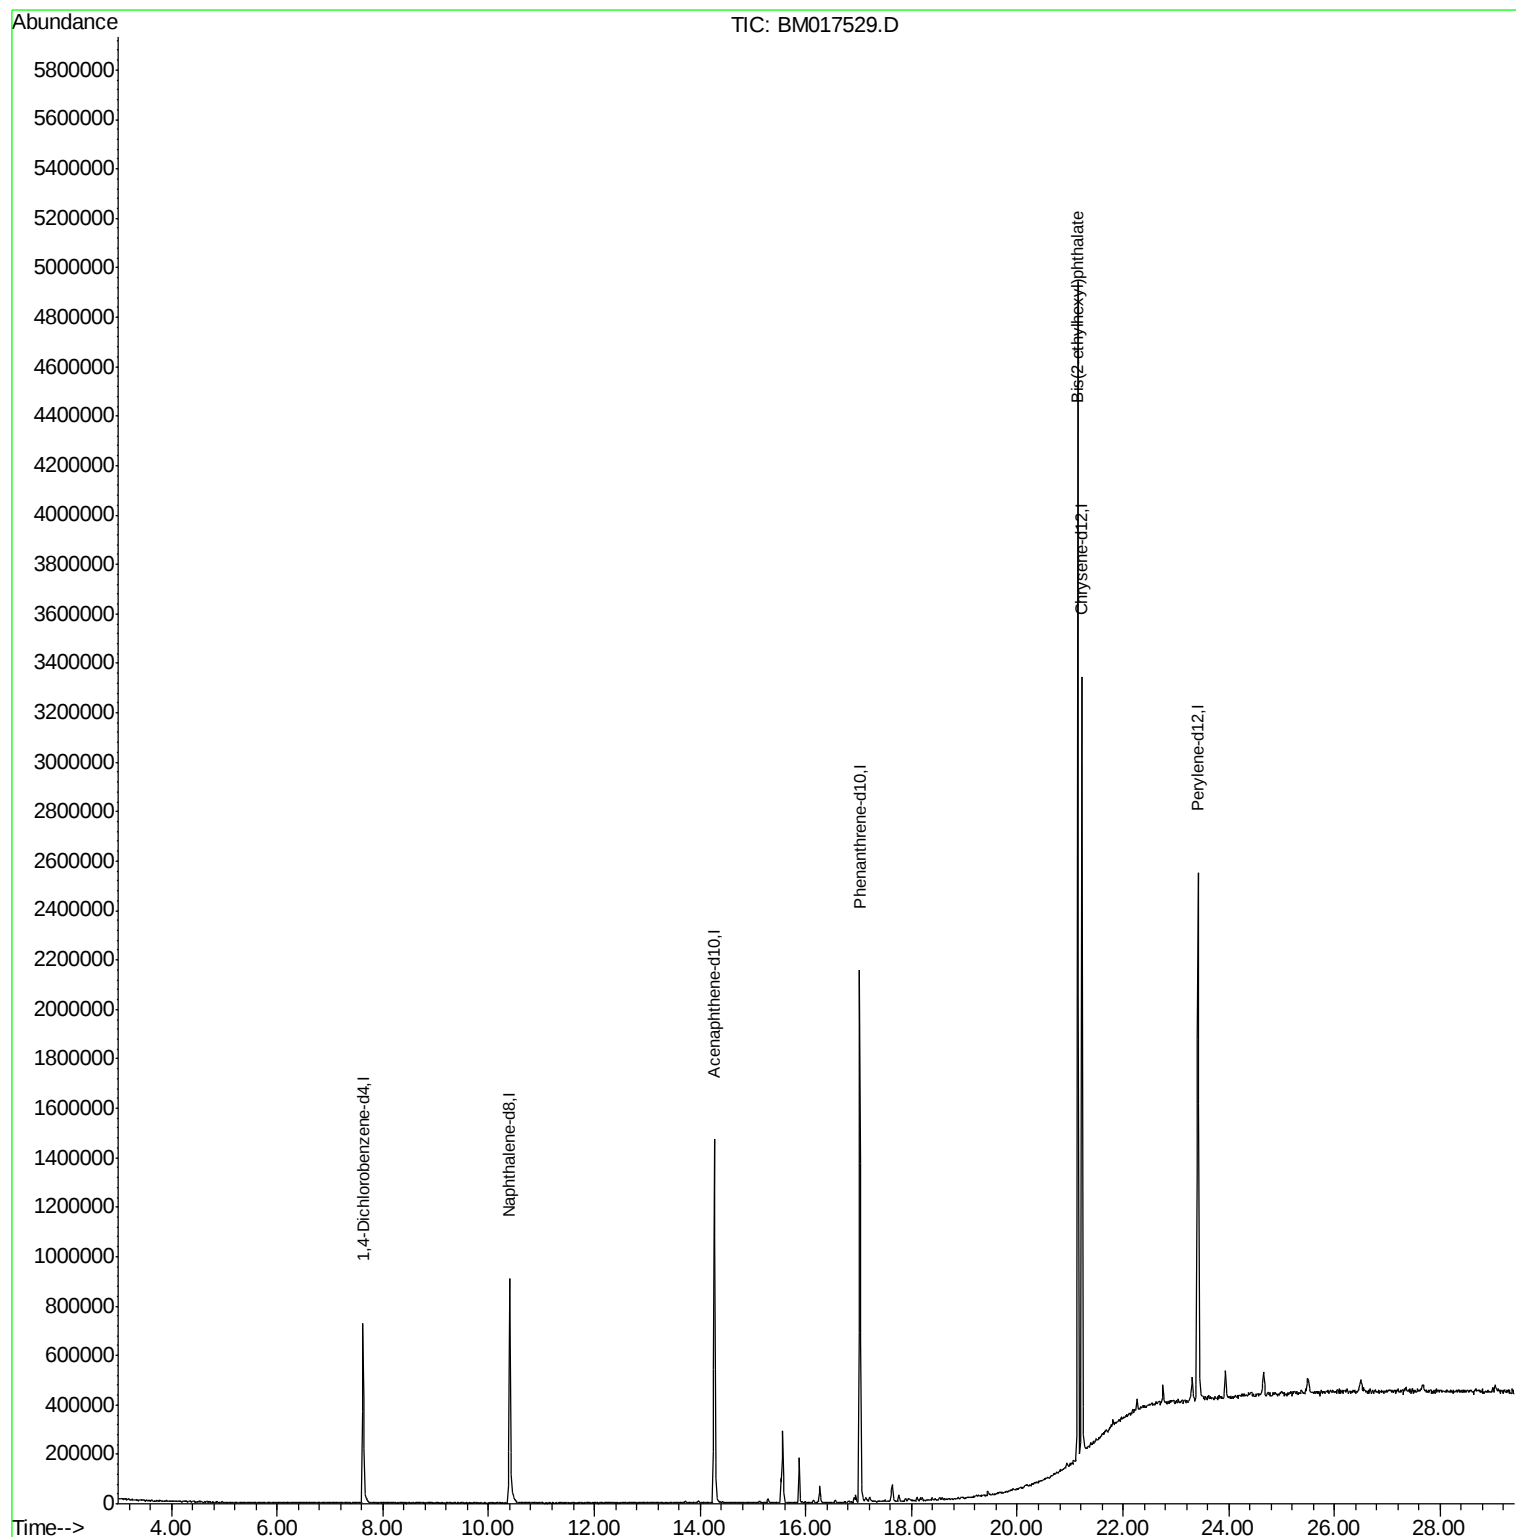

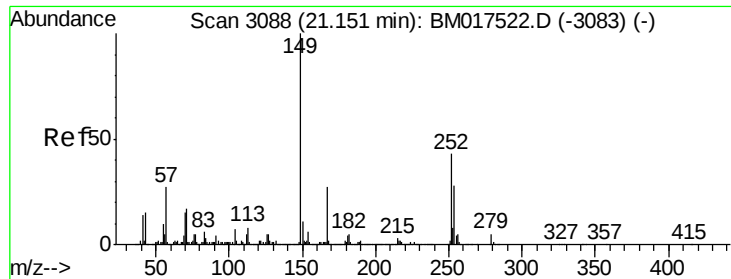

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 29.793 ng/ul
 RT: 21.14 min Scan# 3087
 Delta R.T. -0.01 min
 Lab File: BM017529.D
 Acq: 06 Nov 2018 15:22

Instrument :
 BNA_M
 ClientSampleId :
 A40E4MEDL

Tgt Ion	Ratio	Lower	Upper
149	100		
167	28.1	23.0	34.6
279	4.1	4.1	6.1

Manual Integrations
 APPROVED

Sohil
 11/6/2018 4:36:56 PM

