




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110623\
 Data File : BM042604.D
 Acq On : 07 Nov 2023 00:07
 Operator : MA/JU
 Sample : SSTD3.265
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD3.2013

Manual IntegrationsAPPROVED

Quant Time: Nov 07 02:09:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:04:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/08/2023
 Supervised By :mohammad ahmed 11/08/2023

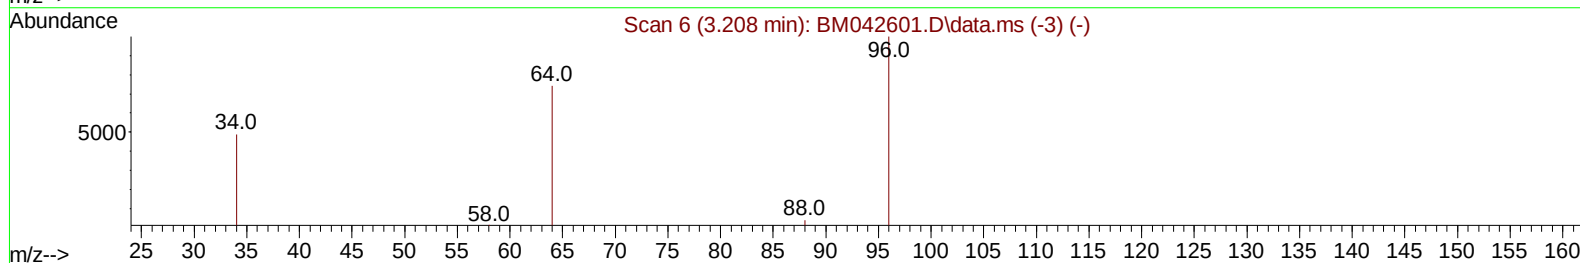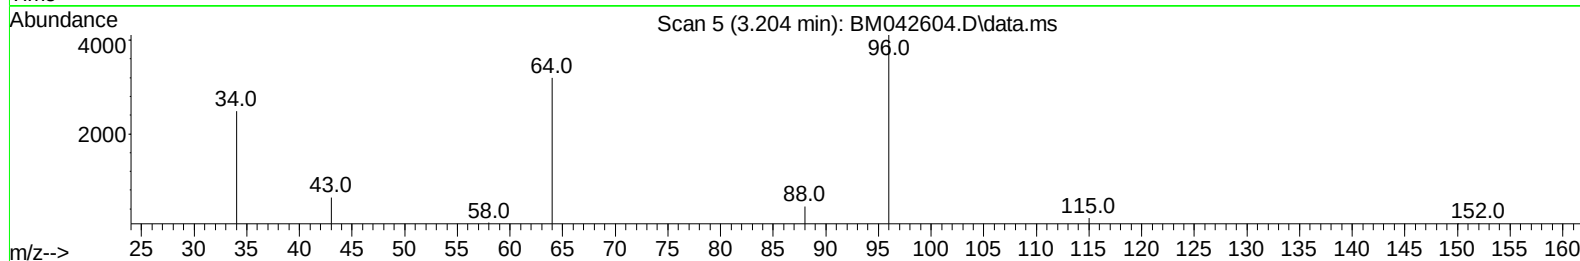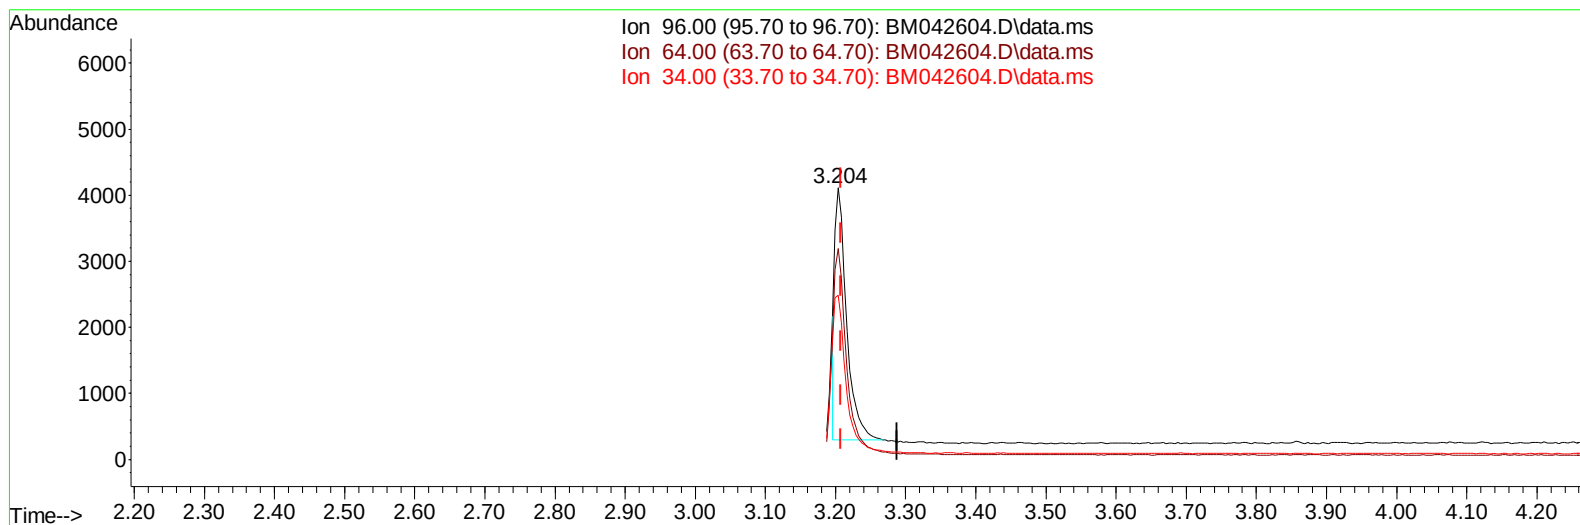

TIC: BM042604.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.204min (-0.004) 2.23 ng/u1

response 4506

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	64.60	77.74#
34.00	55.20	60.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110623\
 Data File : BM042604.D
 Acq On : 07 Nov 2023 00:07
 Operator : MA/JU
 Sample : SSTD3.265
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD3.2013

Manual IntegrationsAPPROVED

Quant Time: Nov 07 02:09:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:04:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/08/2023
 Supervised By :mohammad ahmed 11/08/2023

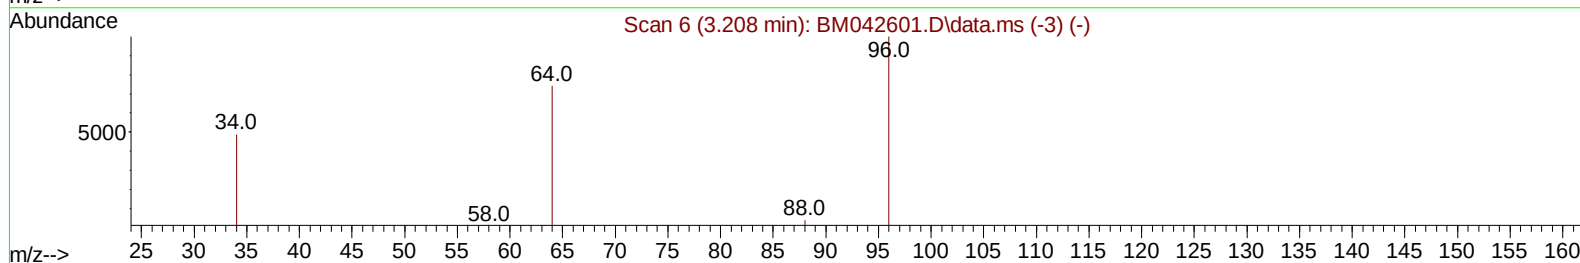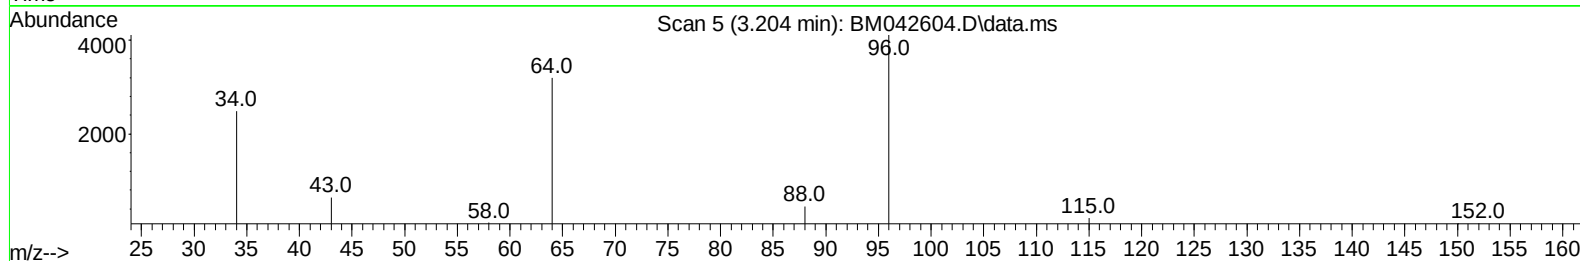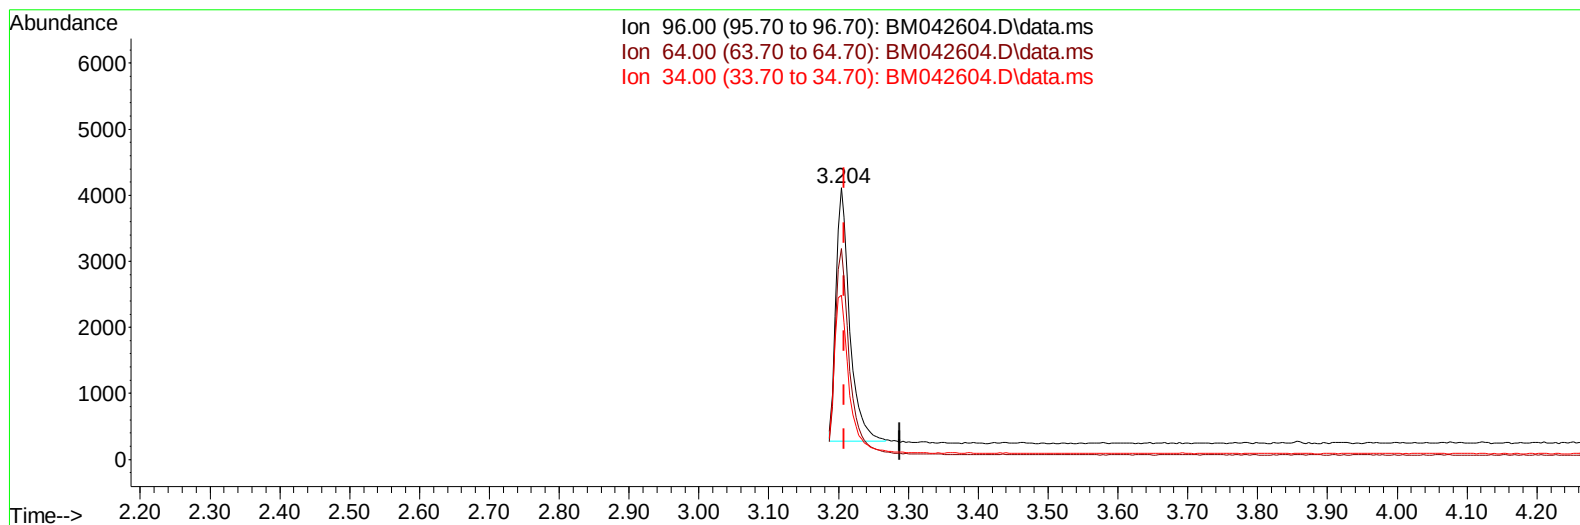

TIC: BM042604.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.204min (-0.004) 2.57 ng/ul m

response 5199

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	64.60	77.74#
34.00	55.20	60.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110623\
 Data File : BM042604.D
 Acq On : 07 Nov 2023 00:07
 Operator : MA/JU
 Sample : SSTD3.265
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD3.2013

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/08/2023
 Supervised By :mohammad ahmed 11/08/2023

Quant Time: Nov 07 02:09:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:04:31 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.870	152		1377	0.400	ng/ul	0.00
4) Naphthalene-d8	10.680	136		3295	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.518	164		2018	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.269	188		4584	0.400	ng/ul	0.00
17) Chrysene-d12	21.451	240		3415	0.400	ng/ul	0.00
23) Perylene-d12	23.839	264		3790	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.204	96		5199m	2.569	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.000	152		0d	0.000	ng/ul	
18) Fluoranthene-d10	0.000	212		0d	0.000	ng/ul	
Target Compounds							Qvalue
2) 1,4-Dioxane	3.242	88		6103	2.637	ng/ul#	59
14) Pentachlorophenol	16.906	266		8197	4.266	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110623\
Data File : BM042604.D
Acq On : 07 Nov 2023 00:07
Operator : MA/JU
Sample : SSTD3.265
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD3.2013

Manual IntegrationsAPPROVED

Quant Time: Nov 07 02:09:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:04:31 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/08/2023
Supervised By :mohammad ahmed 11/08/2023

