


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110718\
 Data File : BM017531.D
 Acq On : 06 Nov 2018 17:42
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 15:08:36 2018

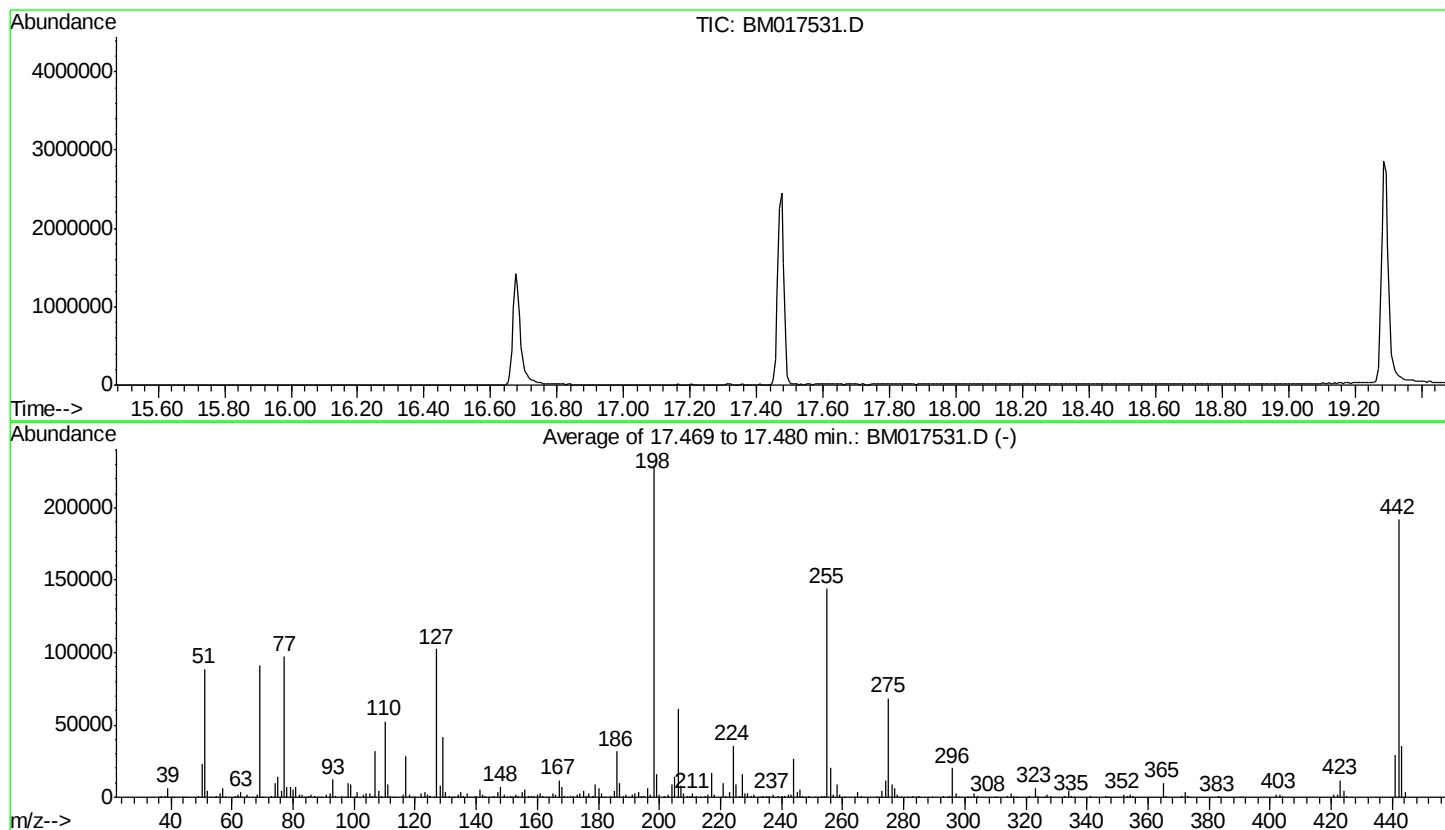

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	88485	PASS
68	69	0.00	2	1.8	1624	PASS
69	198	0.00	100	40.0	91592	PASS
70	69	0.00	2	0.2	187	PASS
127	198	10	80	44.7	102408	PASS
197	198	0.00	2	0.7	1498	PASS
198	198	100	100	100.0	229184	PASS
199	198	5	9	6.8	15633	PASS
275	198	10	60	29.9	68578	PASS
365	198	1	100	4.4	9989	PASS
441	198	0.01	100	12.8	29317	PASS
442	198	50	100	83.7	191765	PASS
443	442	15	24	18.5	35429	PASS