

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042615.D
 Acq On : 07 Nov 2023 16:54
 Operator : MA/JU
 Sample : PB156699BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK699

Quant Time: Nov 07 23:06:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.864	152	1150	0.400	ng/ul	0.00
4) Naphthalene-d8	10.678	136	2897	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.516	164	1672	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.268	188	3752	0.400	ng/ul	0.00
17) Chrysene-d12	21.458	240	2447	0.400	ng/ul	0.00
23) Perylene-d12	23.835	264	3617	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	10087	6.638	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.278	152	1479	0.366	ng/ul	0.00
18) Fluoranthene-d10	19.295	212	3282	0.387	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.511	166	822	0.092	ng/ul#	18
20) Pyrene	19.662	202	820	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.677	252	1465	0.097	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042615.D
Acq On : 07 Nov 2023 16:54
Operator : MA/JU
Sample : PB156699BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK699

Quant Time: Nov 07 23:06:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration




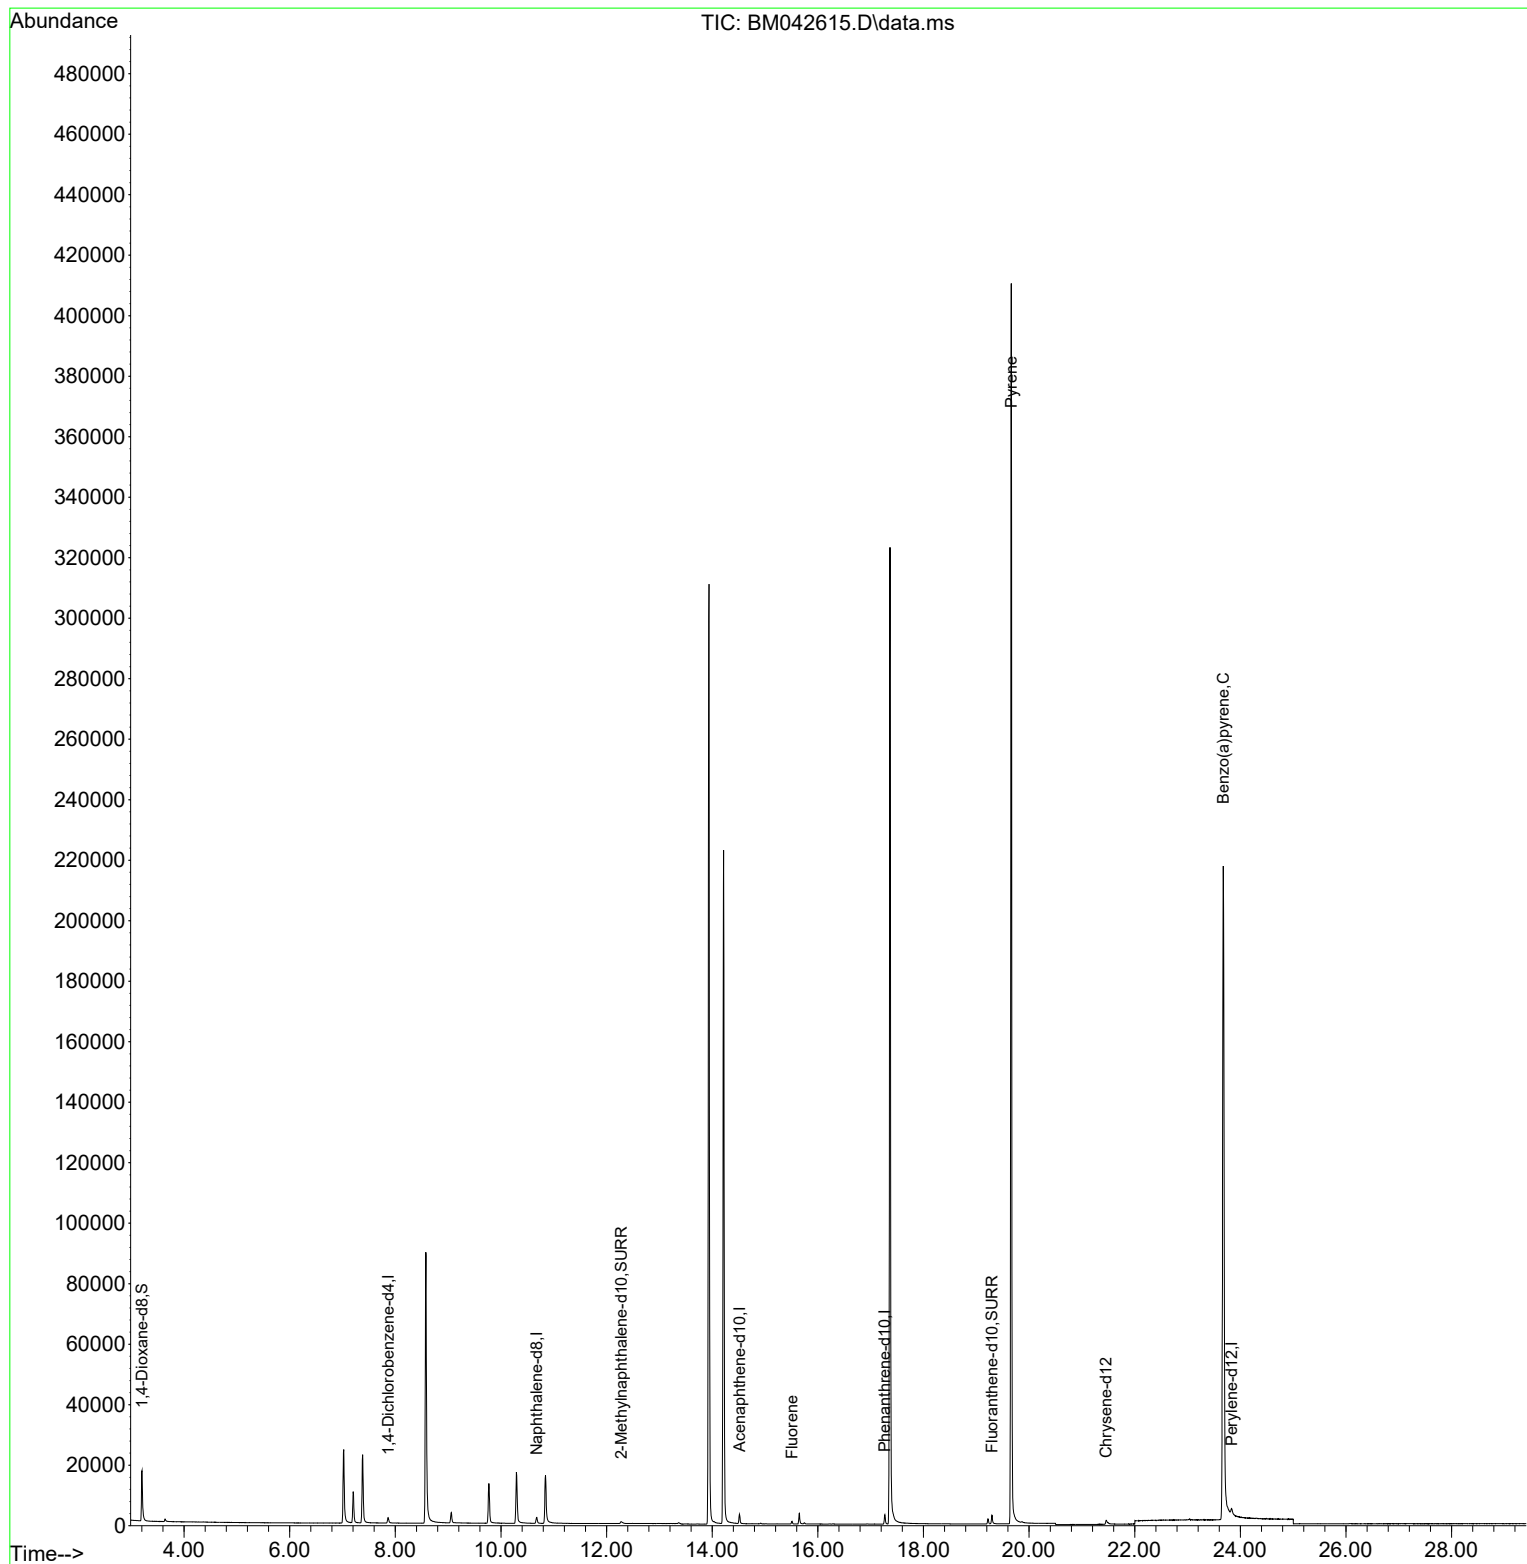


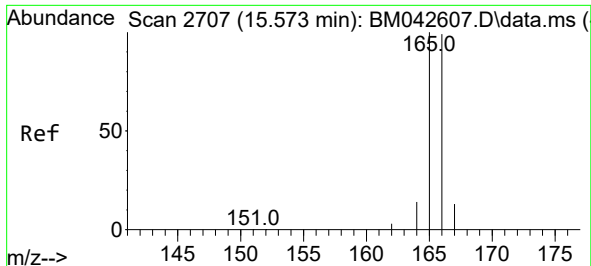

#12
Fluorene
Concen: 0.092 ng/ul
RT: 15.511 min Scan# 21
Delta R.T. -0.058 min
Lab File: BM042615.D
Acq: 07 Nov 2023 16:54




Instrument :
BNA_M
ClientSampleId :
SBLK699


Tgt Ion:166 Resp: 822
Ion Ratio Lower Upper
166 100
165 15.7 81.2 121.8#
167 39.6 11.9 17.9#

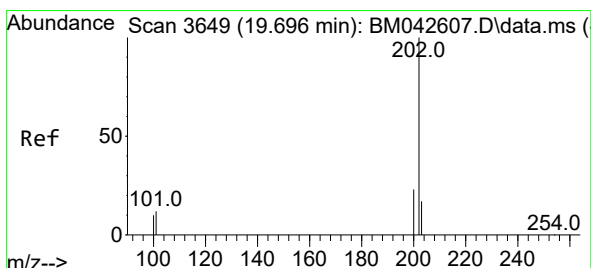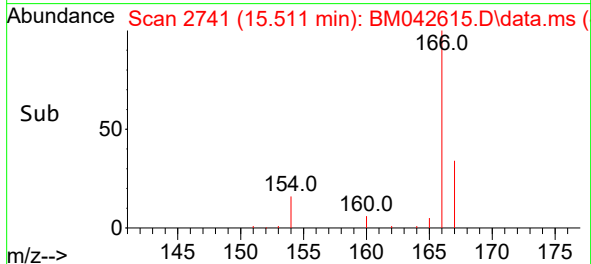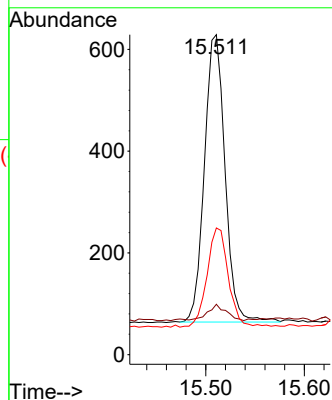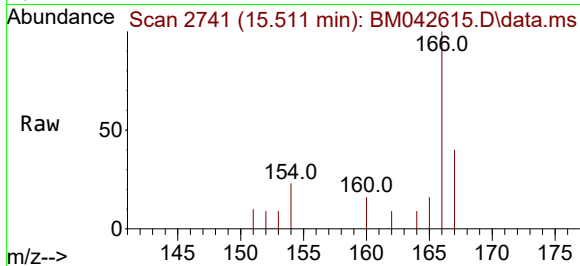

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.662 min Scan# 3689
Delta R.T. -0.034 min
Lab File: BM042615.D
Acq: 07 Nov 2023 16:54


Tgt Ion:202 Resp: 820
Ion Ratio Lower Upper
202 100
101 193.6 10.6 16.0#
100 1473.7 8.6 13.0#

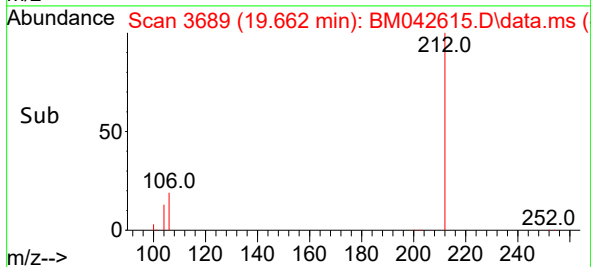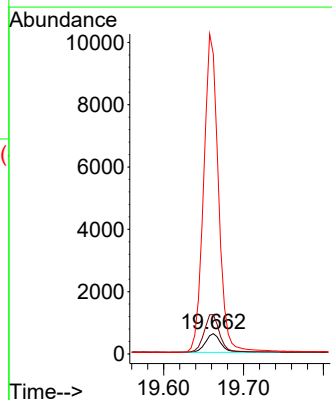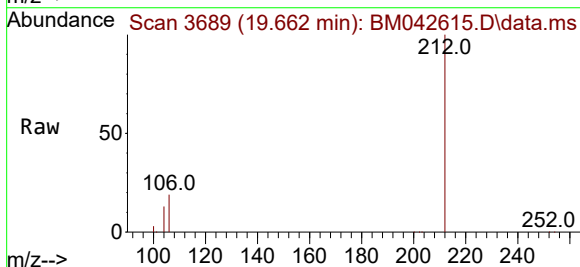

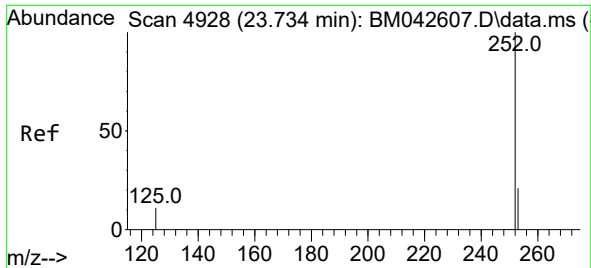

#26
Benzo(a)pyrene
Concen: 0.097 ng/ul
RT: 23.677 min Scan# 49
Delta R.T. -0.057 min
Lab File: BM042615.D
Acq: 07 Nov 2023 16:54

Instrument :
BNA_M
ClientSampleId :
SBLK699

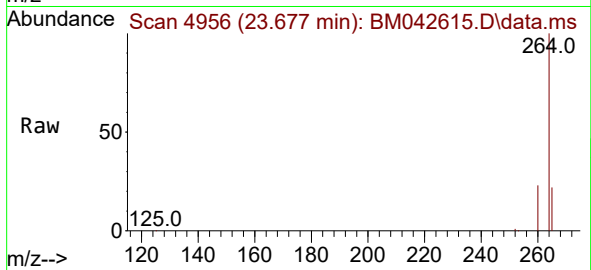

Tgt Ion:252 Resp: 1465
Ion Ratio Lower Upper
252 100
253 61.0 31.7 47.5#
125 48.5 22.1 33.1#

