

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042641.D
 Acq On : 08 Nov 2023 09:09
 Operator : MA/JU
 Sample : 05026-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ6

Quant Time: Nov 08 22:54:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1193	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.671	136	2996	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.510	164	1843	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.262	188	4205	0.400	ng/ul	0.00
17) Chrysene-d12	21.450	240	3131	0.400	ng/ul	0.00
23) Perylene-d12	23.820	264	4742	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.197	96	7923	5.026	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.266	152	1536	0.367	ng/ul	0.00
18) Fluoranthene-d10	19.289	212	3866	0.357	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.505	166	873	0.089	ng/ul#	18
20) Pyrene	19.656	202	901	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.665	252	1563	0.079	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042641.D
Acq On : 08 Nov 2023 09:09
Operator : MA/JU
Sample : 05026-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AJ6

Quant Time: Nov 08 22:54:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration




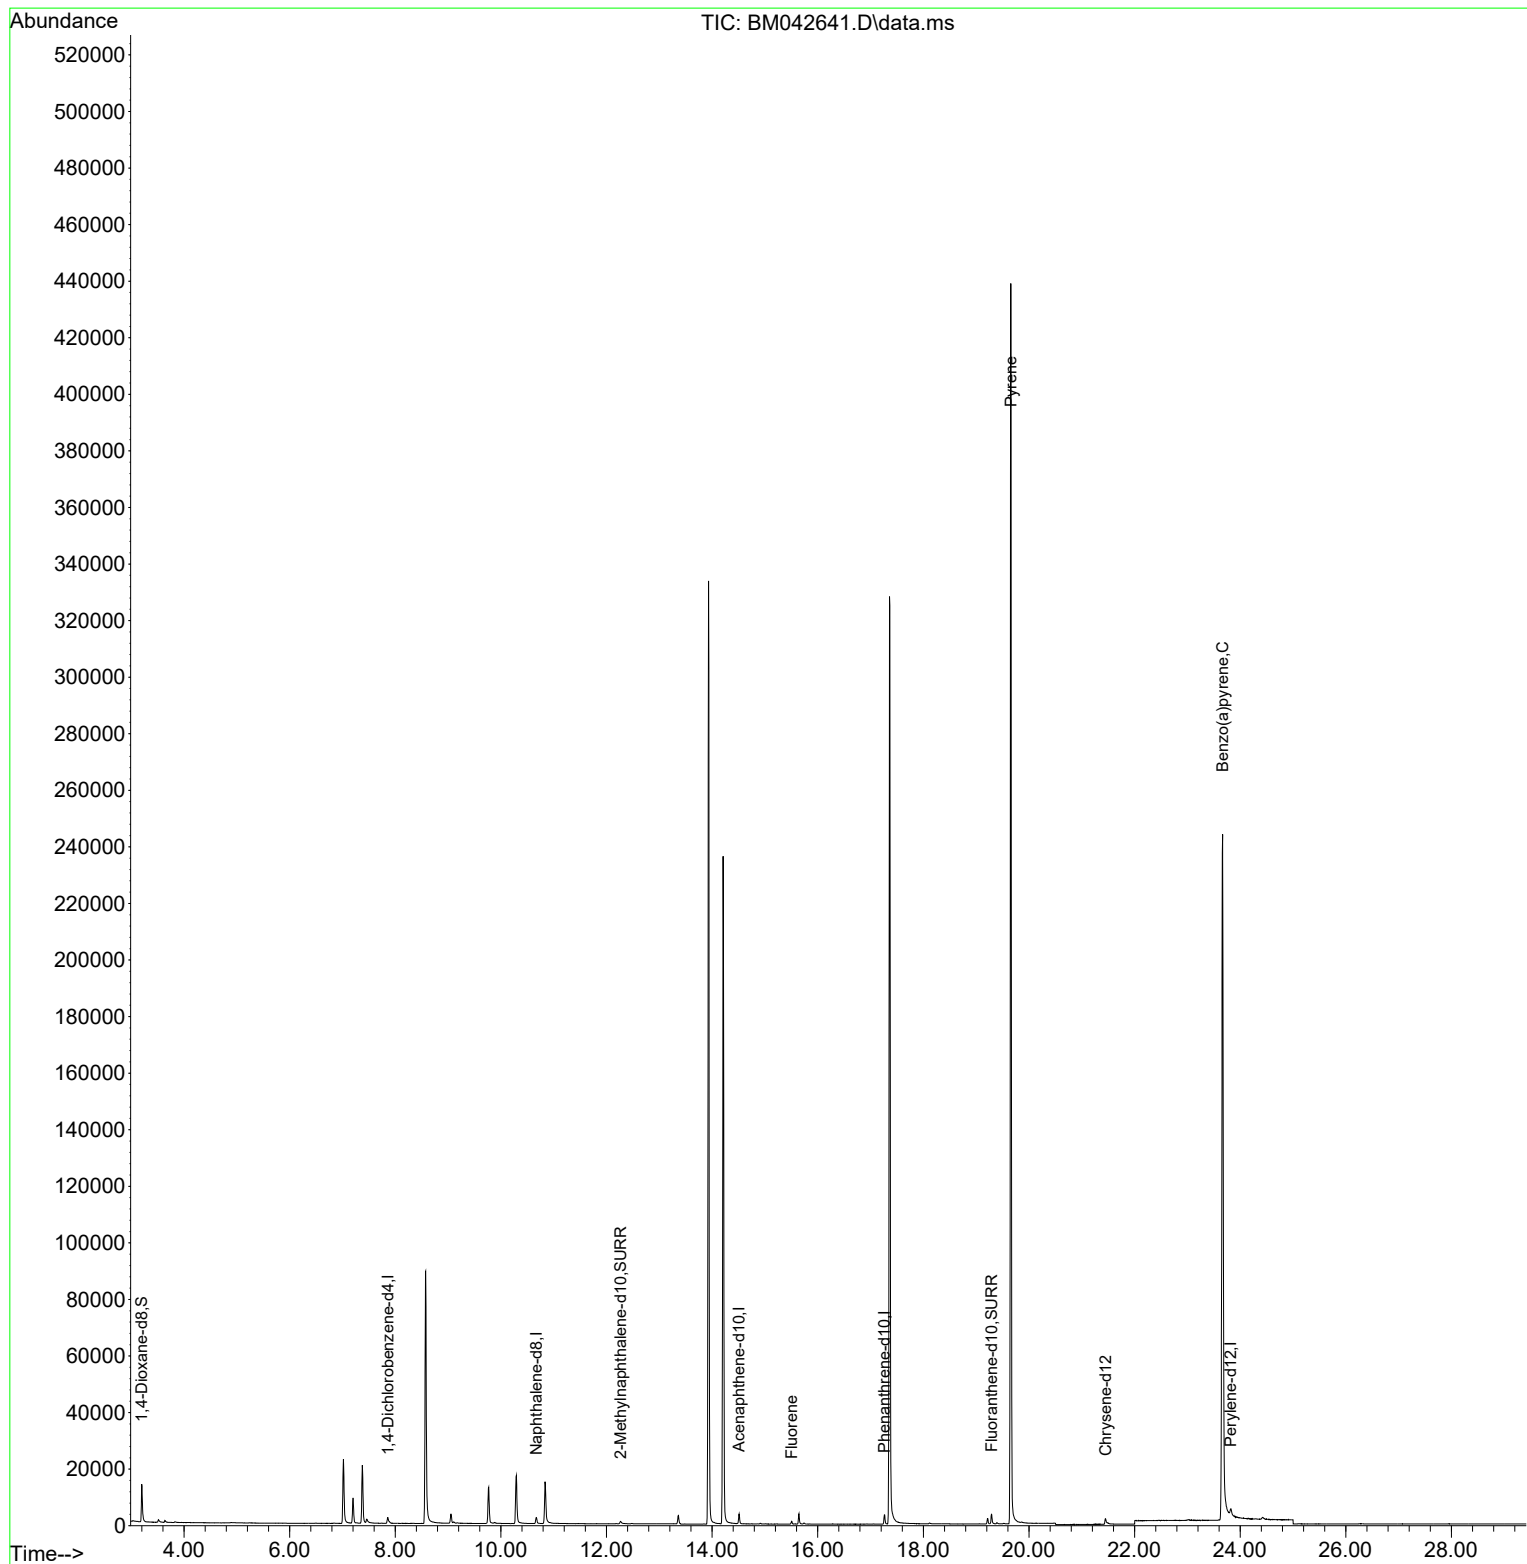


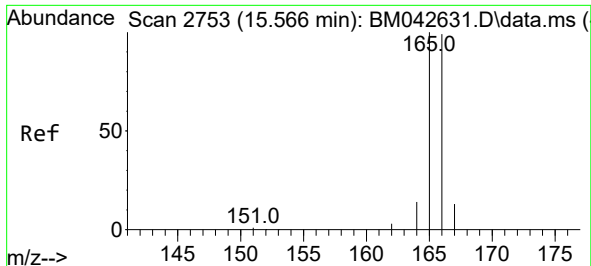

#12
Fluorene
Concen: 0.089 ng/ul
RT: 15.505 min Scan# 21
Delta R.T. -0.064 min
Lab File: BM042641.D
Acq: 08 Nov 2023 09:09




Instrument :
BNA_M
ClientSampleId :
C0AJ6


Tgt Ion:166 Resp: 873
Ion Ratio Lower Upper
166 100
165 14.0 81.2 121.8#
167 36.6 11.9 17.9#

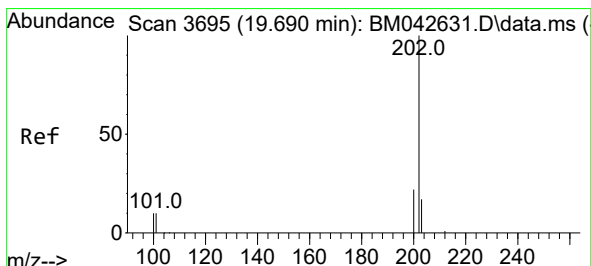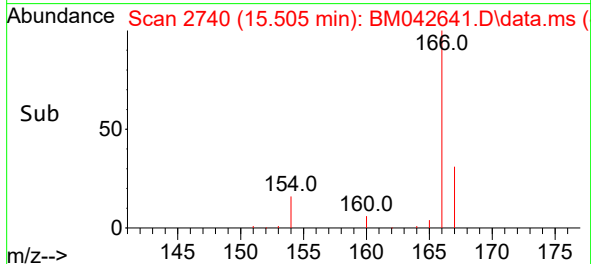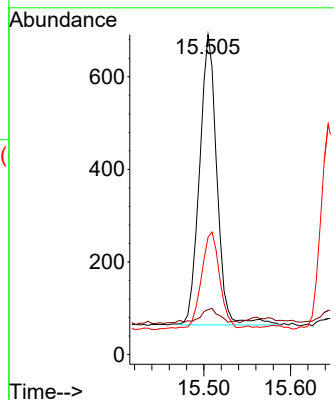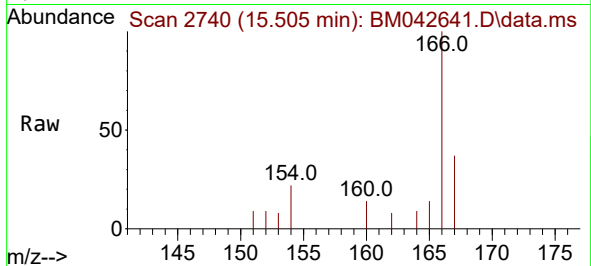

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.656 min Scan# 3688
Delta R.T. -0.040 min
Lab File: BM042641.D
Acq: 08 Nov 2023 09:09


Tgt Ion:202 Resp: 901
Ion Ratio Lower Upper
202 100
101 191.0 10.6 16.0#
100 1450.9 8.6 13.0#

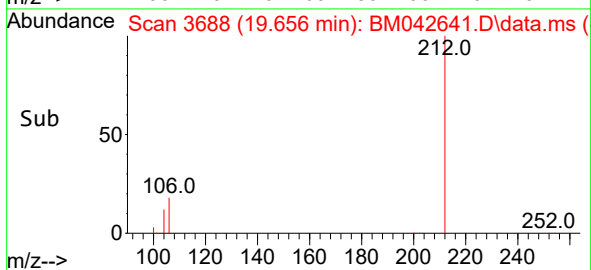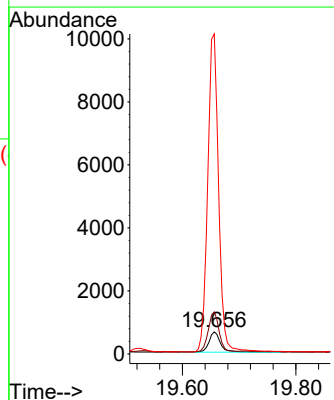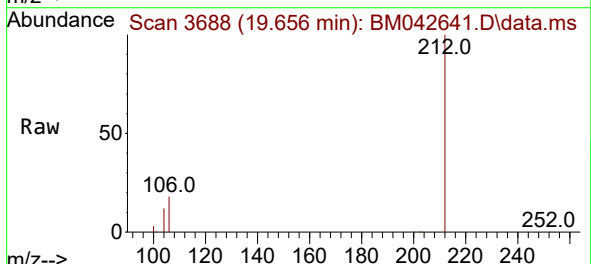

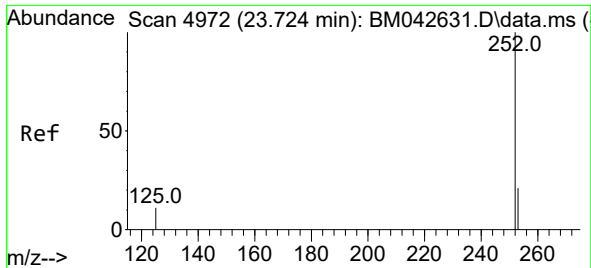

#26
Benzo(a)pyrene
Concen: 0.079 ng/ul
RT: 23.665 min Scan# 4952
Delta R.T. -0.069 min
Lab File: BM042641.D
Acq: 08 Nov 2023 09:09

Instrument :
BNA_M
ClientSampleId :
C0AJ6

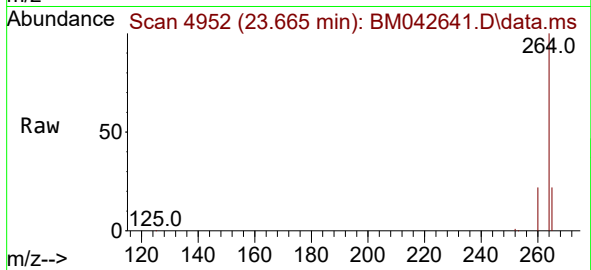

Tgt Ion:252 Resp: 1563
Ion Ratio Lower Upper
252 100
253 60.7 31.7 47.5#
125 50.4 22.1 33.1#

