

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042649.D
 Acq On : 08 Nov 2023 14:58
 Operator : MA/JU
 Sample : PB156630BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 08 22:54:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	1241	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.667	136	2946	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.511	164	1687	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.264	188	3768	0.400	ng/ul	0.00
17) Chrysene-d12	21.455	240	2434	0.400	ng/ul	0.00
23) Perylene-d12	23.826	264	3768	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.198	96	9511	5.800	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.273	152	1188	0.289	ng/ul	0.00
18) Fluoranthene-d10	19.290	212	2659	0.316	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.501	166	735	0.082	ng/ul#	18
20) Pyrene	19.657	202	765	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.665	252	1372	0.087	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042649.D
 Acq On : 08 Nov 2023 14:58
 Operator : MA/JU
 Sample : PB156630BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :


Quant Time: Nov 08 22:54:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

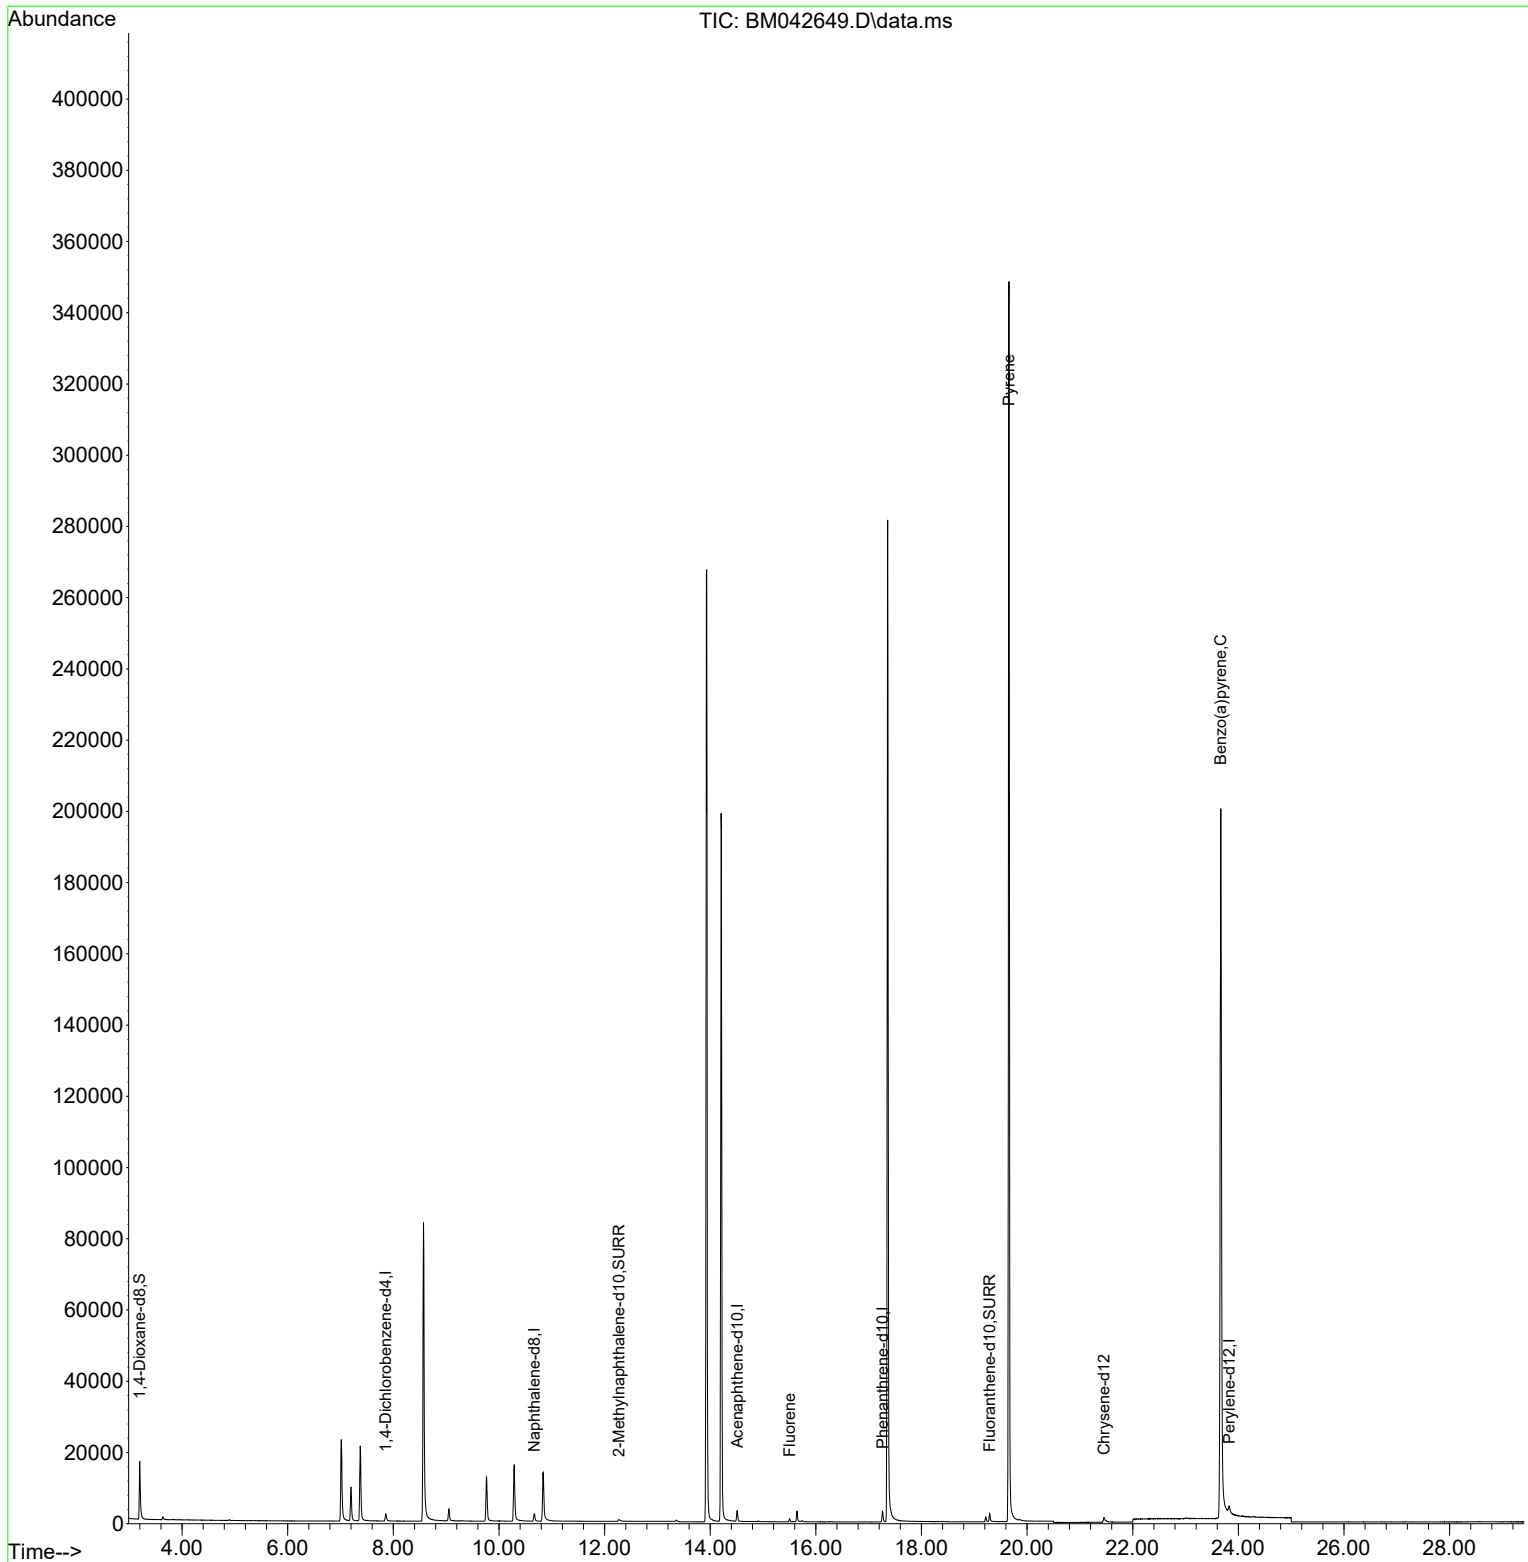



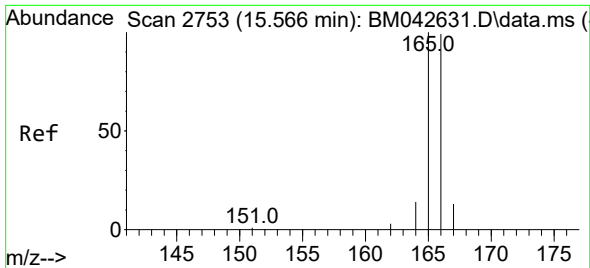


#12
 Fluorene
 Concen: 0.082 ng/u1
 RT: 15.501 min Scan# 21
 Delta R.T. -0.067 min
 Lab File: BM042649.D
 Acq: 08 Nov 2023 14:58


Instrument :
 BNA_M
 ClientSampleId :

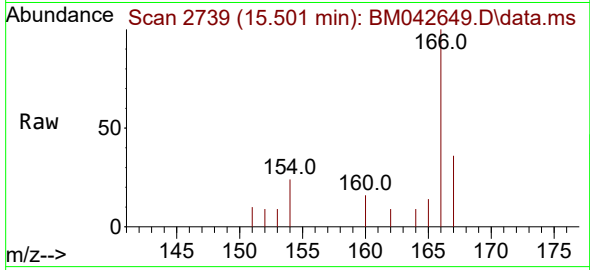



Tgt Ion:166 Resp: 735
 Ion Ratio Lower Upper
 166 100
 165 14.4 81.2 121.8#
 167 36.1 11.9 17.9#

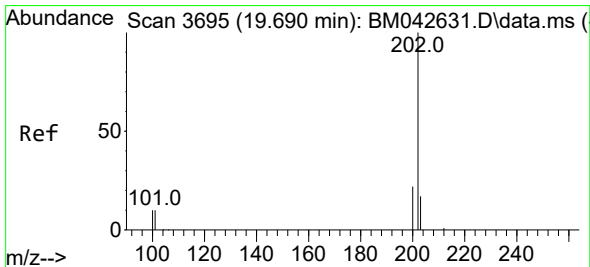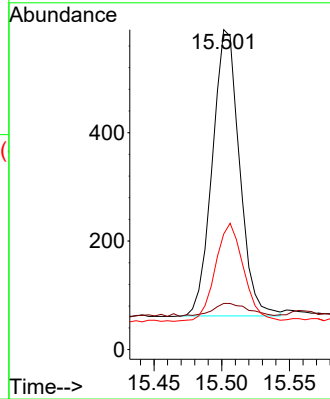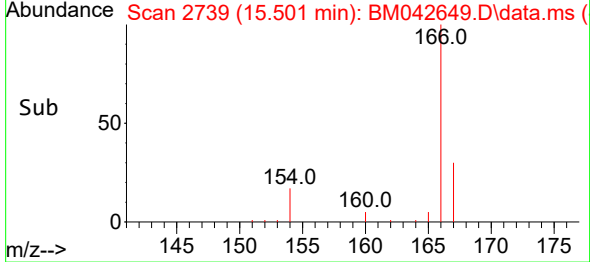


#20
 Pyrene
 Concen: 0.046 ng/u1
 RT: 19.657 min Scan# 3688
 Delta R.T. -0.039 min
 Lab File: BM042649.D
 Acq: 08 Nov 2023 14:58

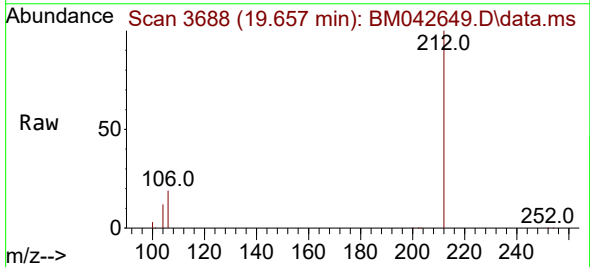


Tgt Ion:202 Resp: 765
 Ion Ratio Lower Upper
 202 100
 101 195.0 10.6 16.0#
 100 1476.2 8.6 13.0#

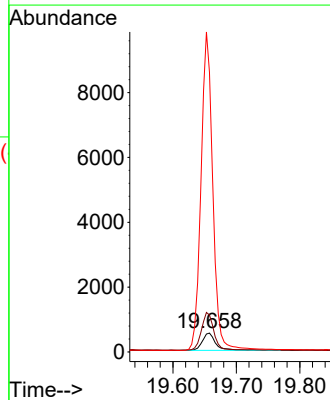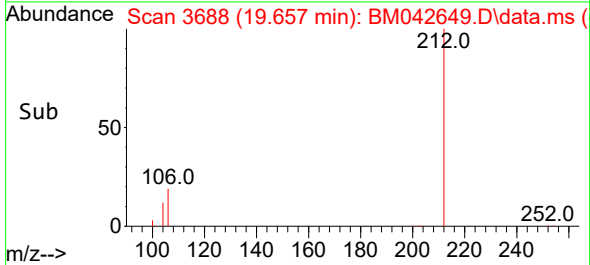

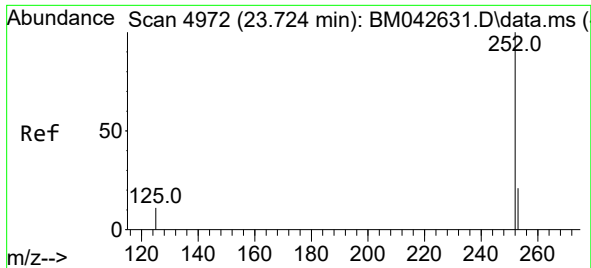

#26
 Benzo(a)pyrene
 Concen: 0.087 ng/ul
 RT: 23.665 min Scan# 4952
 Delta R.T. -0.069 min
 Lab File: BM042649.D
 Acq: 08 Nov 2023 14:58

Instrument :
 BNA_M
 ClientSampleId :

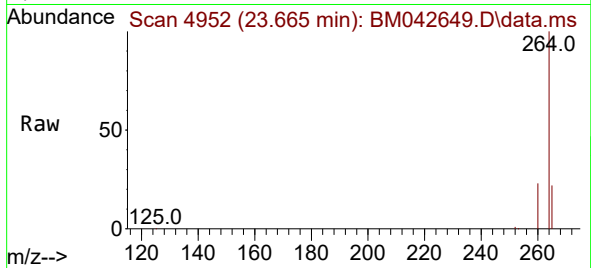

Tgt Ion:252 Resp: 1372
 Ion Ratio Lower Upper
 252 100
 253 56.0 31.7 47.5#
 125 42.6 22.1 33.1#

