

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042651.D
 Acq On : 08 Nov 2023 16:10
 Operator : MA/JU
 Sample : 04948-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK2

Quant Time: Nov 08 22:55:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.855	152	1156	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.667	136	2738	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.507	164	1561	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.264	188	3441	0.400	ng/ul	0.00
17) Chrysene-d12	21.452	240	2368	0.400	ng/ul	0.00
23) Perylene-d12	23.820	264	3347	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.198	96	7317	4.790	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.267	152	1090	0.285	ng/ul	0.00
18) Fluoranthene-d10	19.290	212	2534	0.309	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.657	202	789	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.668	252	1210	0.086	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042651.D
Acq On : 08 Nov 2023 16:10
Operator : MA/JU
Sample : 04948-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK2

Quant Time: Nov 08 22:55:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration




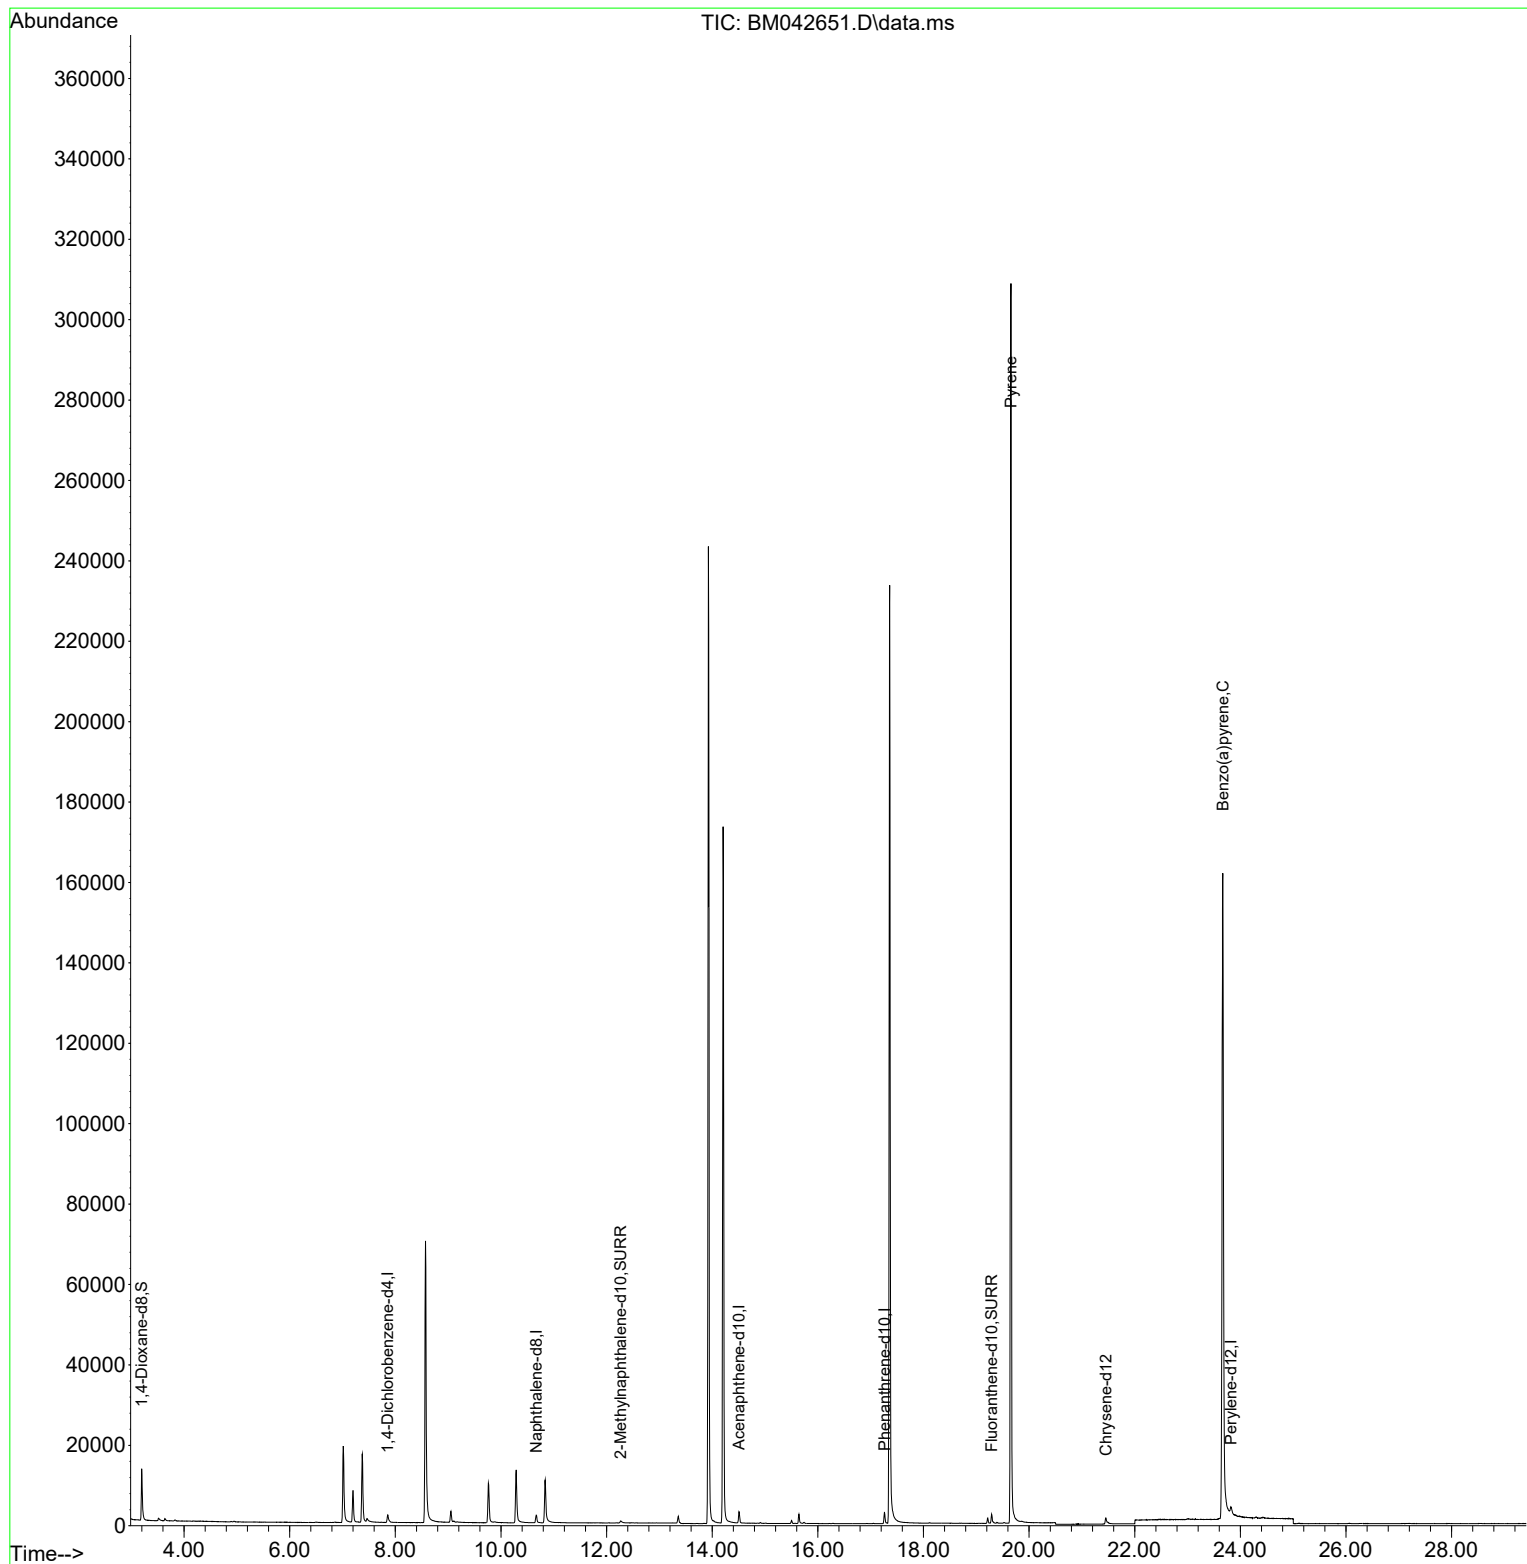


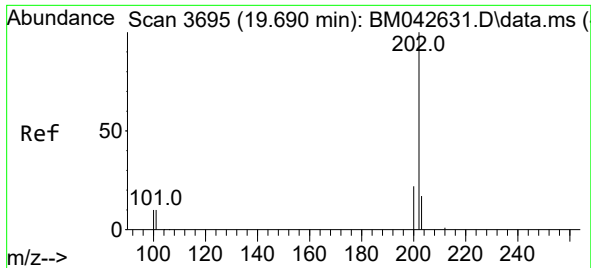

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.657 min Scan# 3688
Delta R.T. -0.039 min
Lab File: BM042651.D
Acq: 08 Nov 2023 16:10

Instrument :
BNA_M
ClientSampleId :
C0AK2

Tgt Ion:202 Resp: 789
Ion Ratio Lower Upper
202 100
101 189.9 10.6 16.0#
100 1408.6 8.6 13.0#

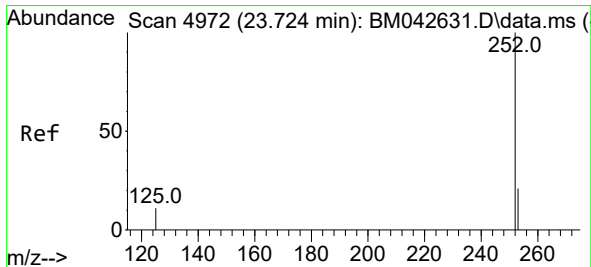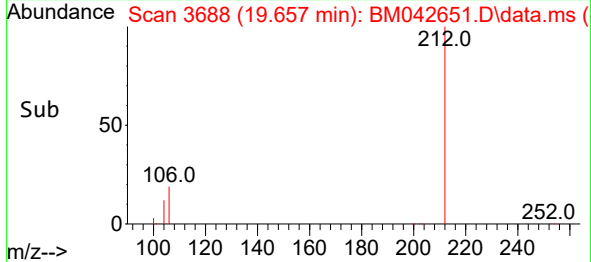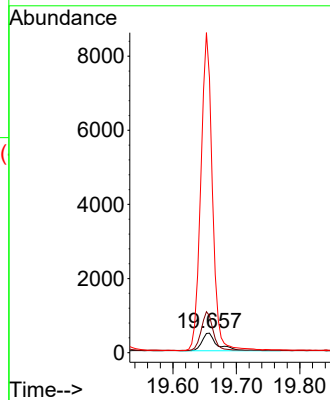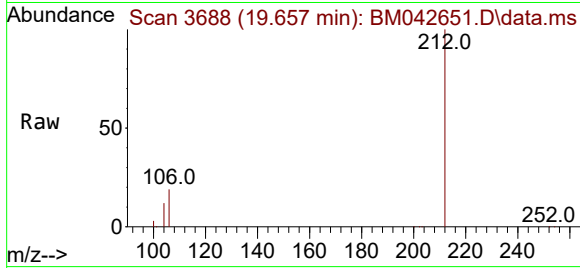

#26
Benzo(a)pyrene
Concen: 0.086 ng/ul
RT: 23.668 min Scan# 4953
Delta R.T. -0.066 min
Lab File: BM042651.D
Acq: 08 Nov 2023 16:10

Tgt Ion:252 Resp: 1210
Ion Ratio Lower Upper
252 100
253 62.1 31.7 47.5#
125 49.1 22.1 33.1#

