

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042659.D
 Acq On : 08 Nov 2023 20:59
 Operator : MA/JU
 Sample : 05158-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH366

Quant Time: Nov 08 22:56:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1196	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.667	136	2783	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.507	164	1510	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.260	188	3343	0.400	ng/ul	-0.01
17) Chrysene-d12	21.447	240	2362	0.400	ng/ul	0.00
23) Perylene-d12	23.823	264	3177	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.198	96	5238	3.314	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.262	152	460	0.118	ng/ul	-0.01
18) Fluoranthene-d10	19.290	212	1359	0.166	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.240	88	318	0.169	ng/ul#	72
26) Benzo(a)pyrene	23.665	252	653	0.049	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042659.D
Acq On : 08 Nov 2023 20:59
Operator : MA/JU
Sample : 05158-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH366

Quant Time: Nov 08 22:56:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration




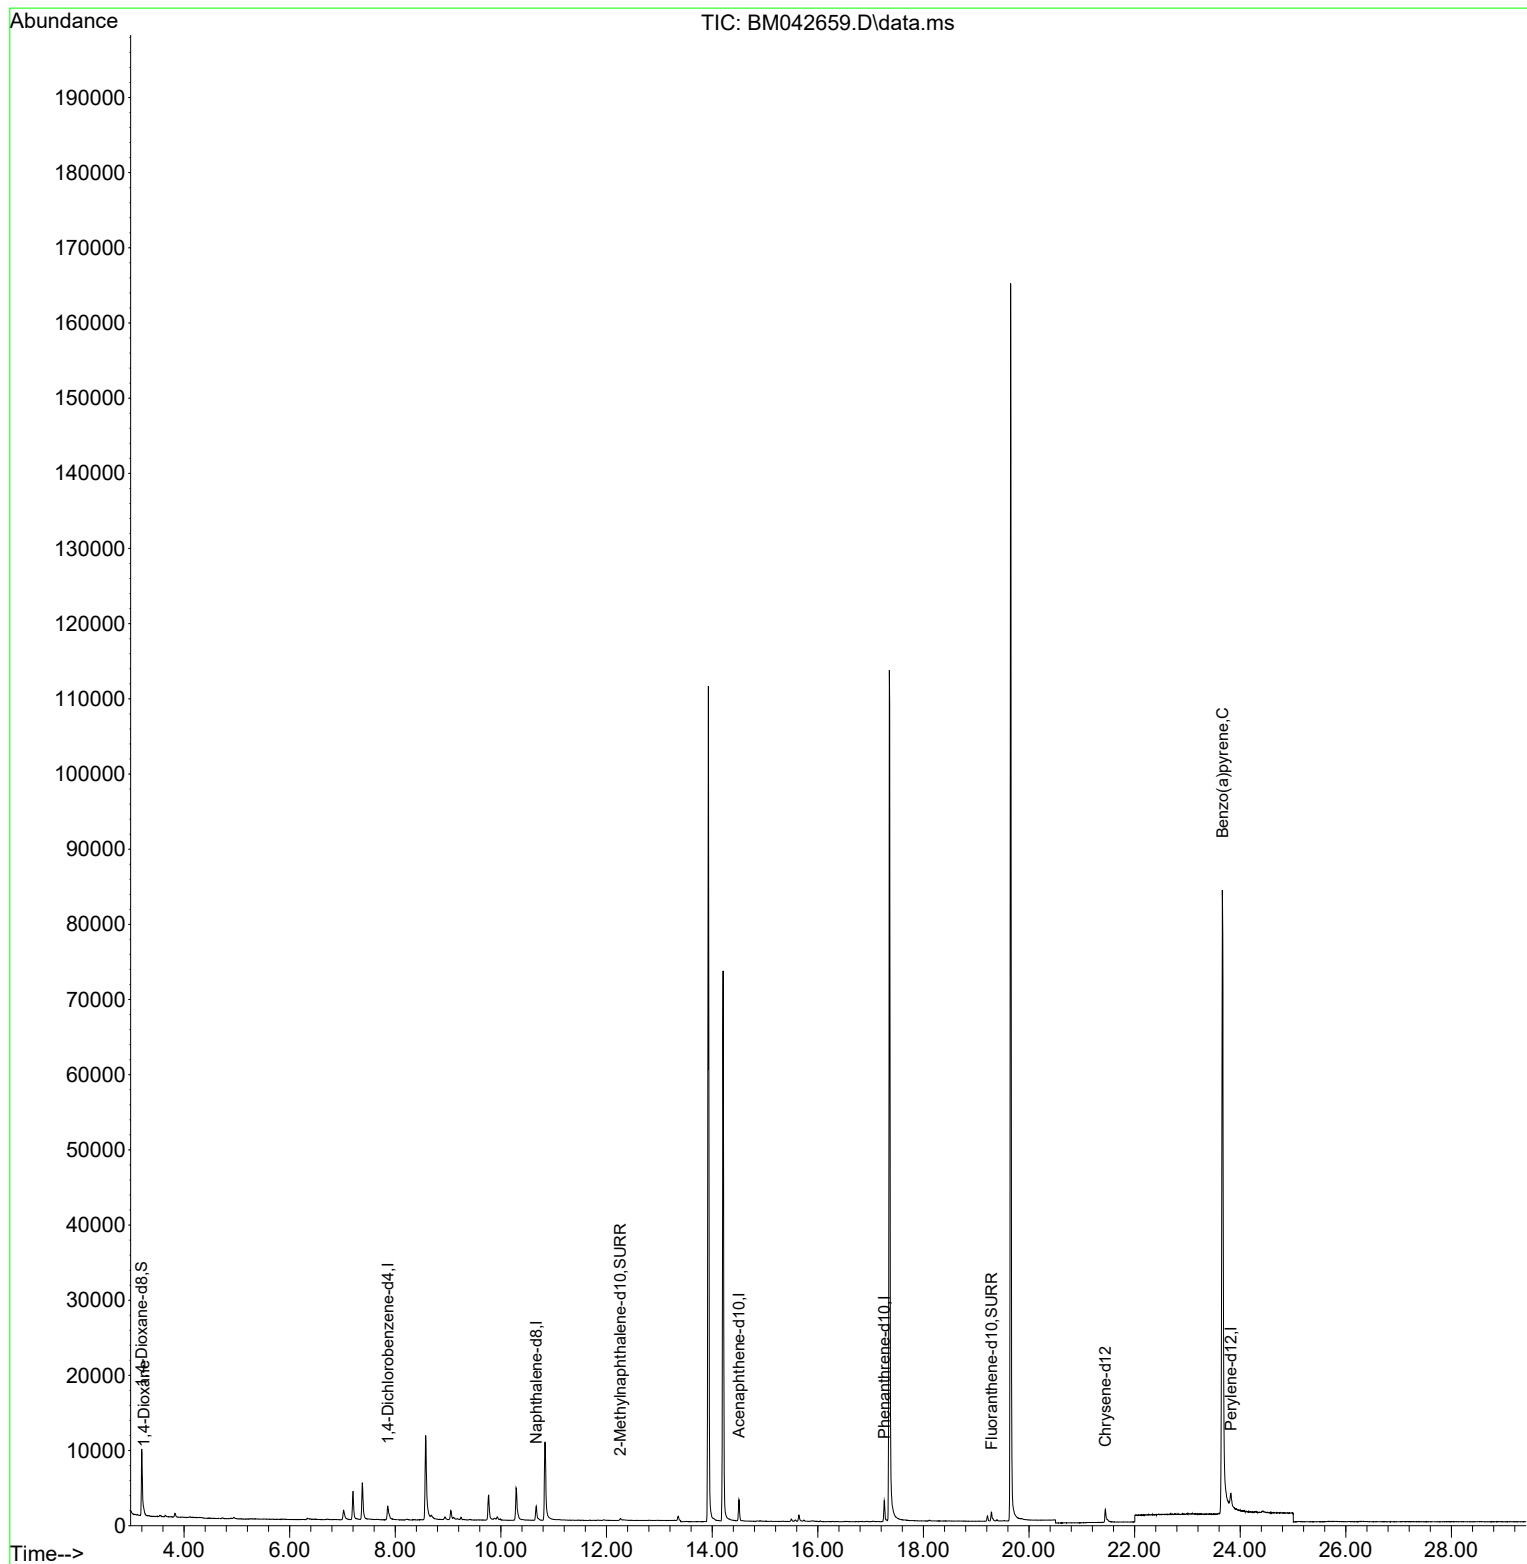


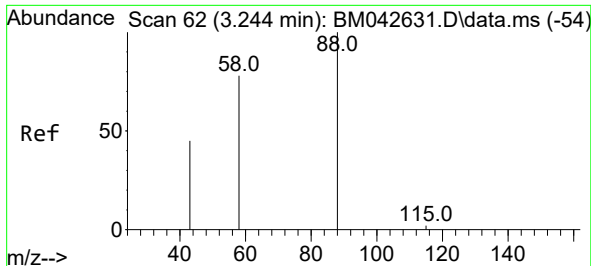

#2
1,4-Dioxane
Concen: 0.169 ng/ul
RT: 3.240 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM042659.D
Acq: 08 Nov 2023 20:59

Instrument :
BNA_M
ClientSampleId :
BH366

Tgt Ion: 88 Resp: 318
Ion Ratio Lower Upper
88 100
43 65.5 77.5 116.3#
58 36.5 40.9 61.3#

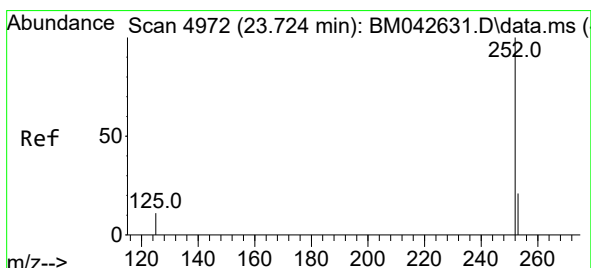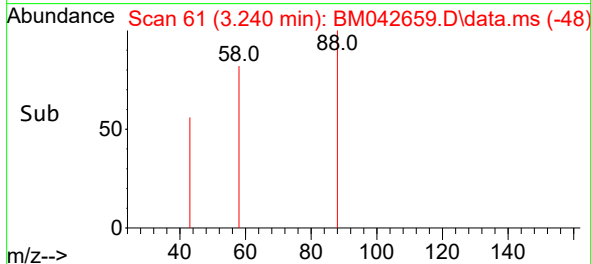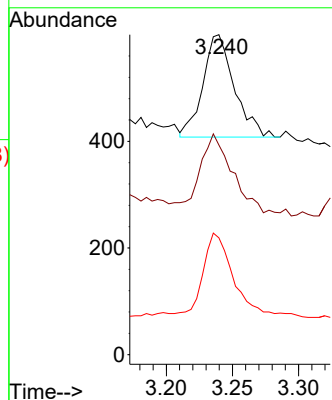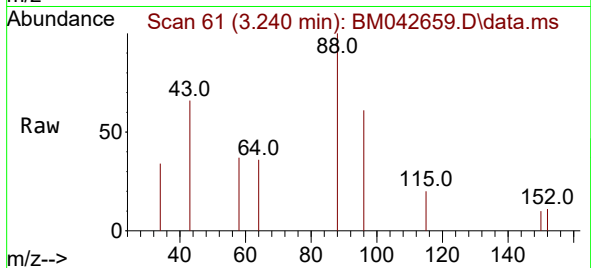

#26
Benzo(a)pyrene
Concen: 0.049 ng/ul
RT: 23.665 min Scan# 4952
Delta R.T. -0.069 min
Lab File: BM042659.D
Acq: 08 Nov 2023 20:59

Tgt Ion: 252 Resp: 653
Ion Ratio Lower Upper
252 100
253 80.3 31.7 47.5#
125 61.1 22.1 33.1#

