




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042608.D
Acq On : 07 Nov 2023 09:26
Operator : MA/JU
Sample : PB156842BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK842

Manual IntegrationsAPPROVED

Quant Time: Nov 07 23:05:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :mohammad ahmed 11/09/2023

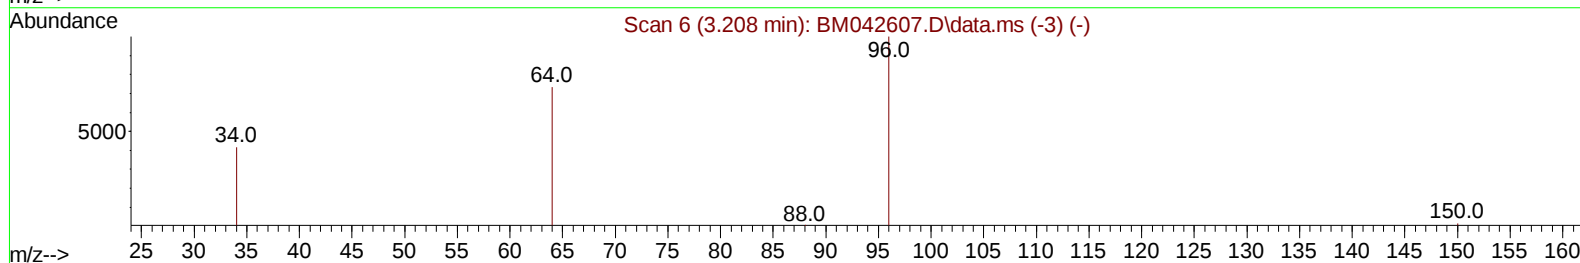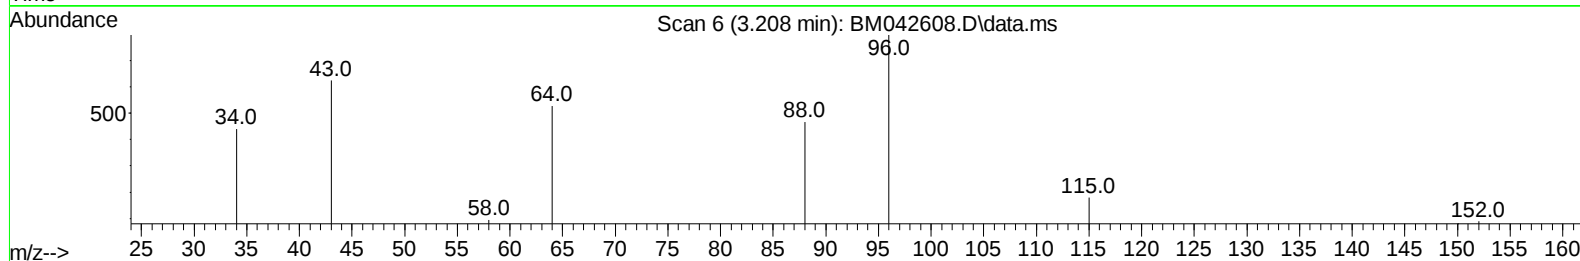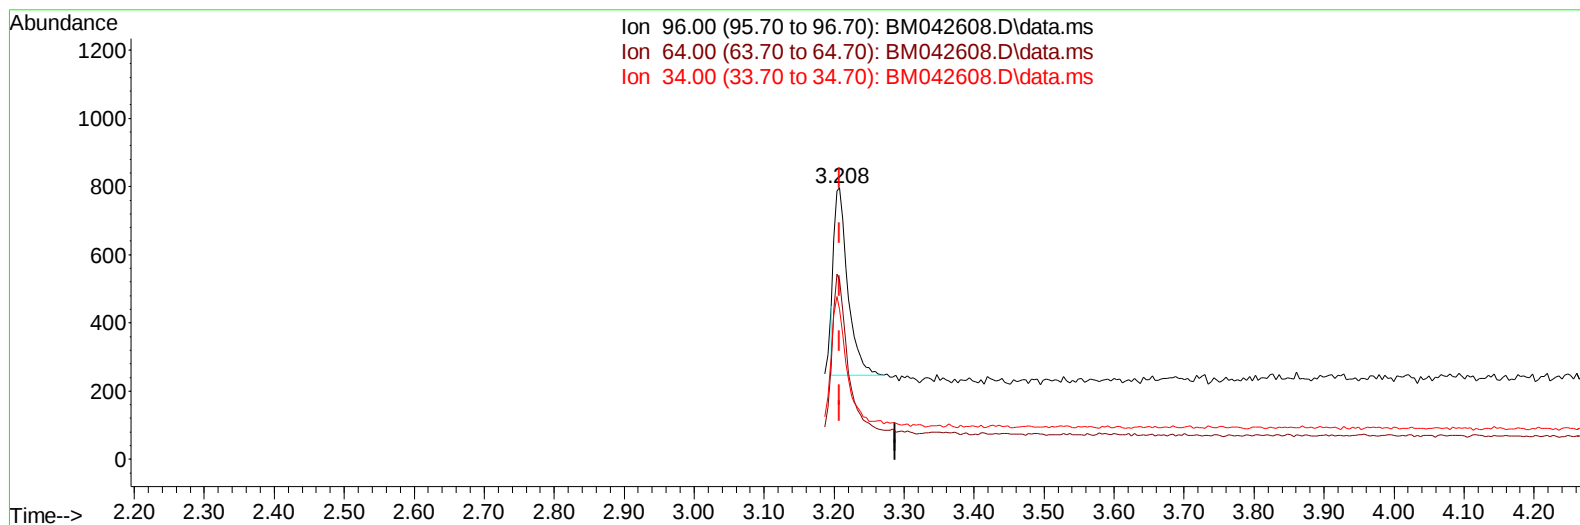

TIC: BM042608.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.208min (-0.000) 0.59 ng/u1

response 761

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	64.60	66.21
34.00	55.20	55.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042608.D
 Acq On : 07 Nov 2023 09:26
 Operator : MA/JU
 Sample : PB156842BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK842

Manual IntegrationsAPPROVED

Quant Time: Nov 07 23:05:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/09/2023

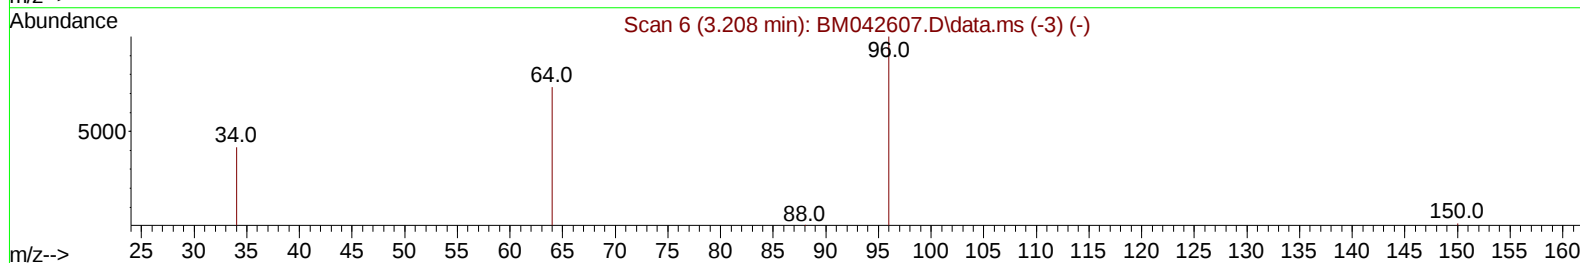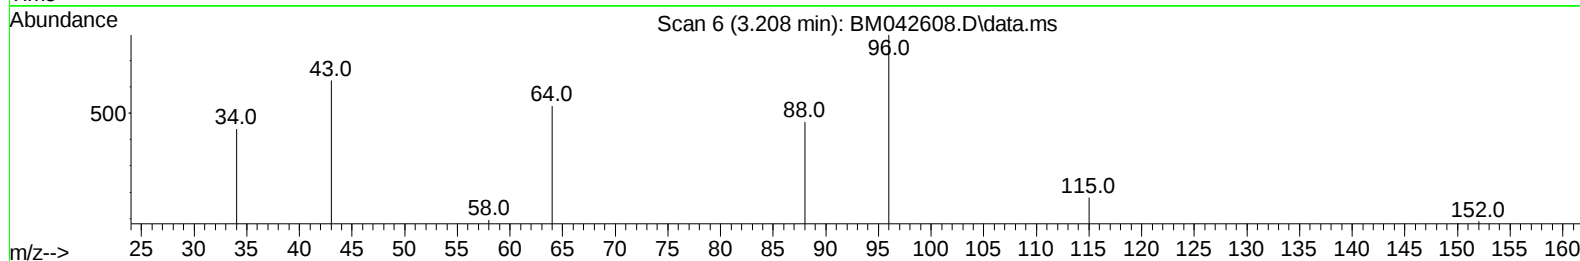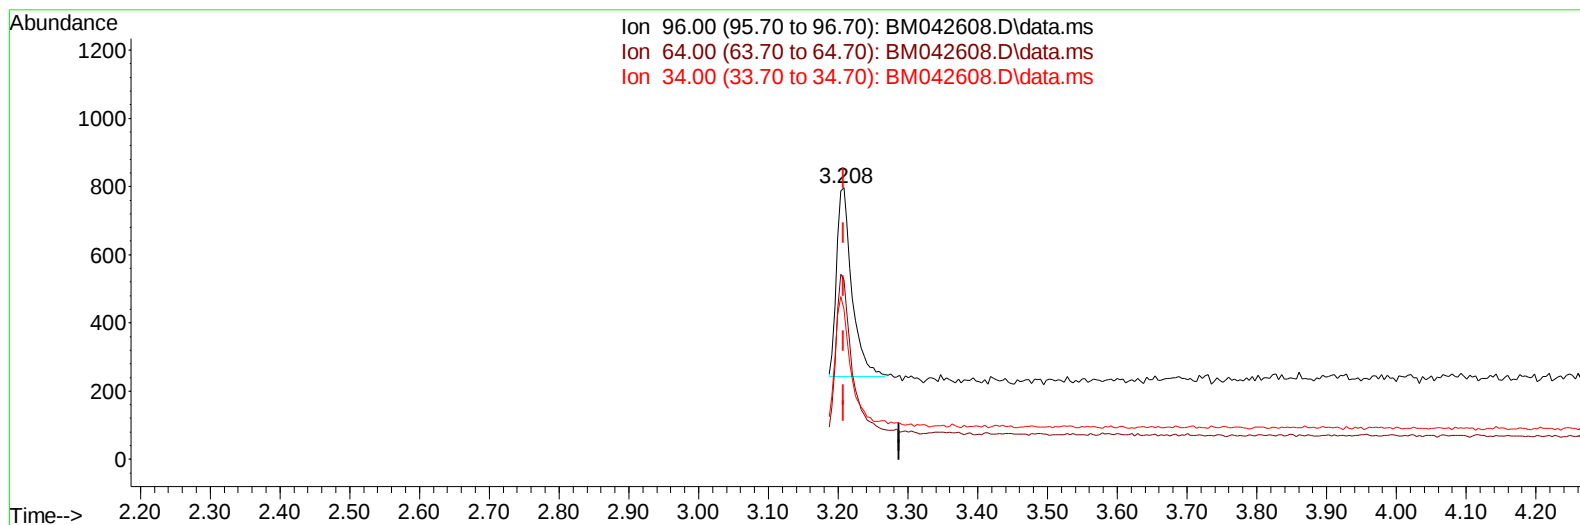

TIC: BM042608.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.208min (-0.000) 0.66 ng/ul m

response 847

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	64.60	66.21
34.00	55.20	55.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042608.D
 Acq On : 07 Nov 2023 09:26
 Operator : MA/JU
 Sample : PB156842BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK842

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/09/2023

Quant Time: Nov 07 23:05:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.882	152	971	0.400	ng/ul	0.01
4) Naphthalene-d8	10.697	136	2279	0.400	ng/ul #	0.02
9) Acenaphthene-d10	14.518	164	1365	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.278	188	2609	0.400	ng/ul	0.00
17) Chrysene-d12	21.457	240	2147	0.400	ng/ul	0.00
23) Perylene-d12	23.842	264	2535	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.208	96	847m	0.660	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.286	152	973	0.306	ng/ul	0.01
18) Fluoranthene-d10	19.301	212	2593	0.349	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042608.D
Acq On : 07 Nov 2023 09:26
Operator : MA/JU
Sample : PB156842BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK842

Manual IntegrationsAPPROVED

Quant Time: Nov 07 23:05:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :mohammad ahmed 11/09/2023

