




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042633.D
 Acq On : 08 Nov 2023 04:21
 Operator : MA/JU
 Sample : PB156701BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK701

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/09/2023

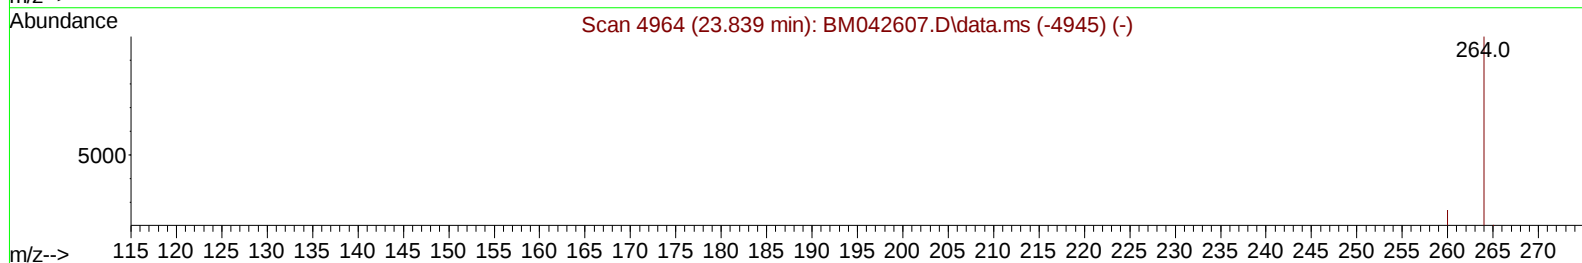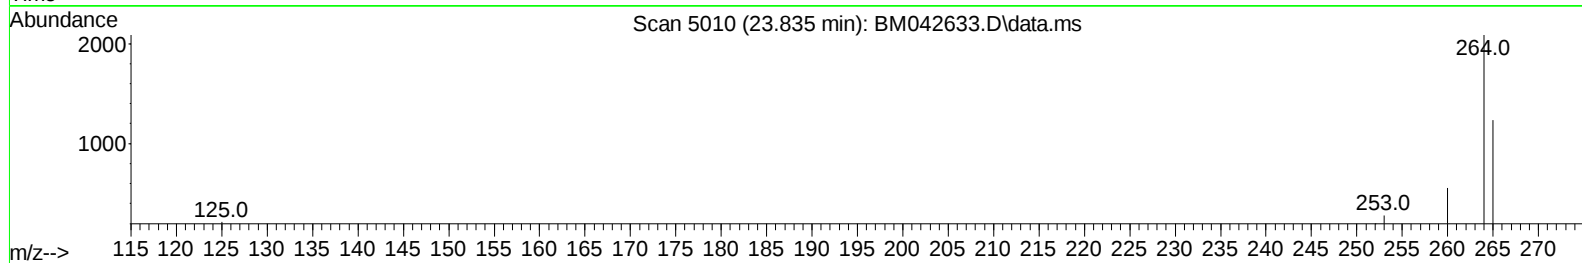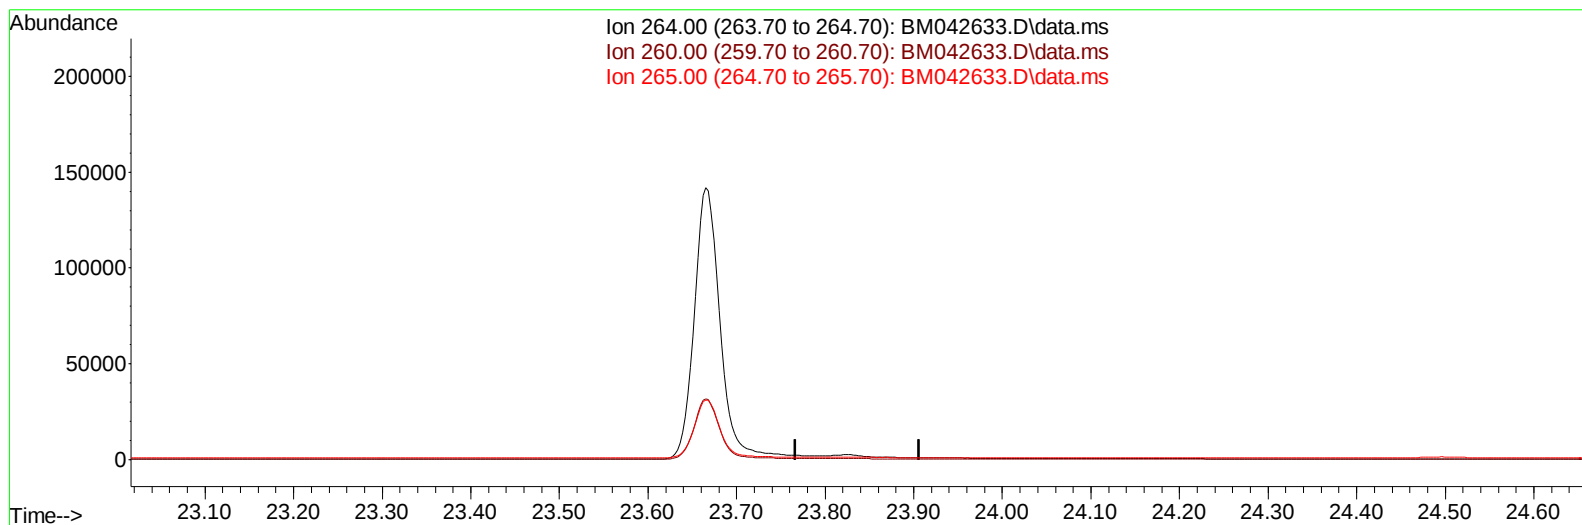

TIC: BM042633.D\data.ms

(23) Perylene-d12 (I)

23.836min (-23.836) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	30.50	0.00#
265.00	107.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042633.D
 Acq On : 08 Nov 2023 04:21
 Operator : MA/JU
 Sample : PB156701BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK701

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/09/2023

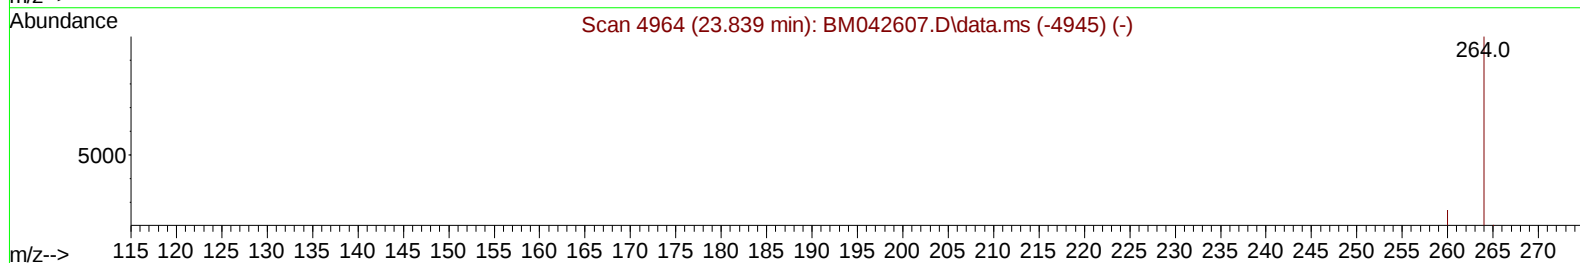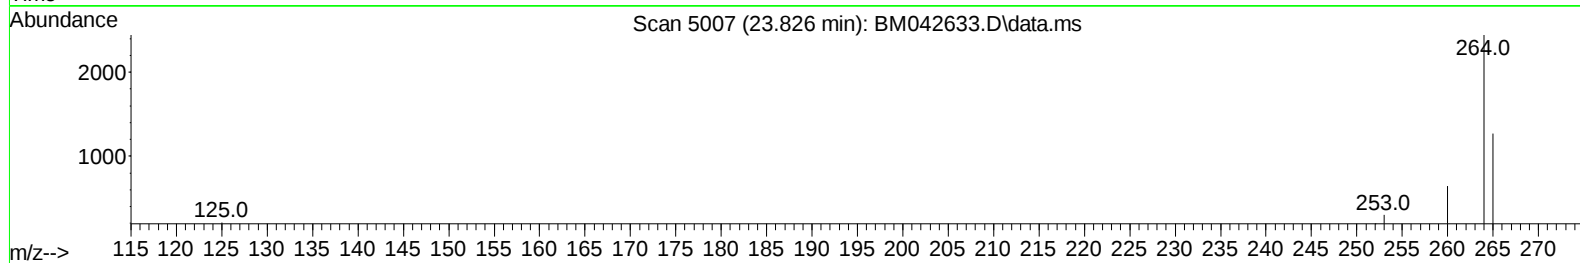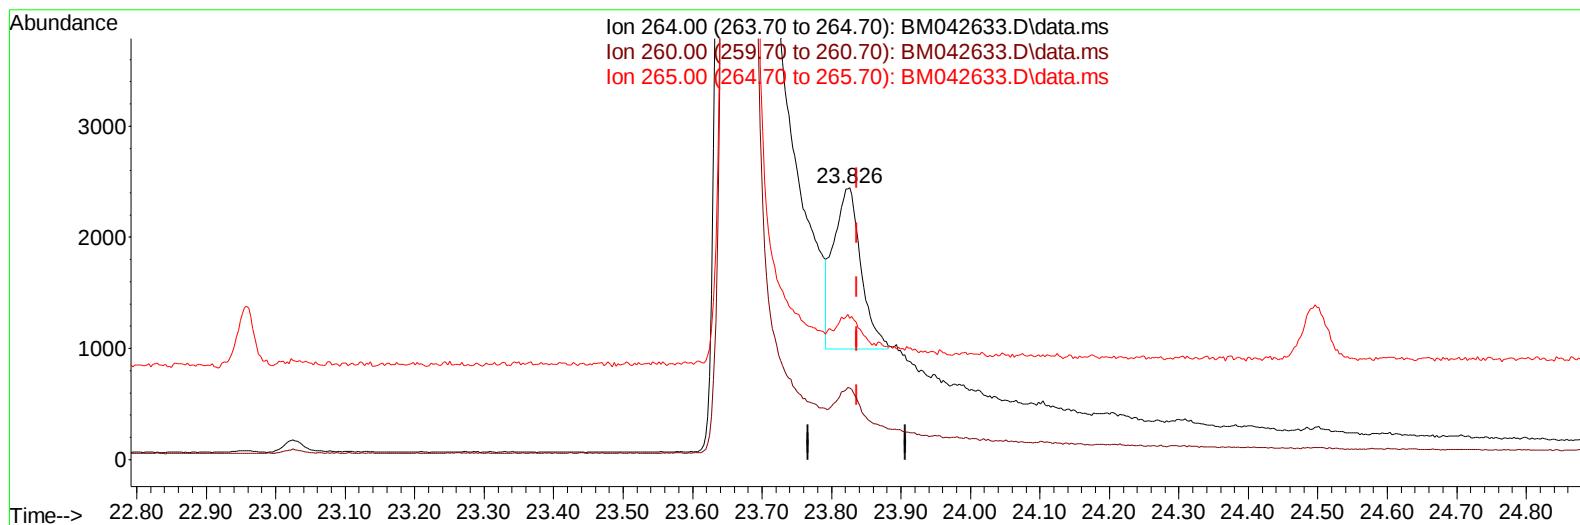

TIC: BM042633.D\data.ms

(23) Perylene-d12 (I)

23.826min (-0.010) 0.40 ng/ul m

response 3978

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	30.50	26.43
265.00	107.10	52.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042633.D
 Acq On : 08 Nov 2023 04:21
 Operator : MA/JU
 Sample : PB156701BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK701

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :mohammad ahmed 11/09/2023

Quant Time: Nov 08 04:52:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1106	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.671	136	2715	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.515	164	1646	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.267	188	3700	0.400	ng/ul	0.00
17) Chrysene-d12	21.453	240	2341	0.400	ng/ul	0.00
23) Perylene-d12	23.826	264	3978m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	9018	6.170	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.271	152	1341	0.354	ng/ul	0.00
18) Fluoranthene-d10	19.294	212	3027	0.373	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042633.D
Acq On : 08 Nov 2023 04:21
Operator : MA/JU
Sample : PB156701BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK701

Manual IntegrationsAPPROVED

Quant Time: Nov 08 04:52:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :mohammad ahmed 11/09/2023

