

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042616.D
 Acq On : 07 Nov 2023 17:30
 Operator : MA/JU
 Sample : 05026-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH328

Quant Time: Nov 07 23:06:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.864	152	1148	0.400	ng/ul	0.00
4) Naphthalene-d8	10.677	136	2743	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.515	164	1731	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.267	188	4073	0.400	ng/ul	0.00
17) Chrysene-d12	21.453	240	2735	0.400	ng/ul	0.00
23) Perylene-d12	23.832	264	3655	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	6307	4.157	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.266	152	1617	0.422	ng/ul	0.00
18) Fluoranthene-d10	19.294	212	4553	0.481	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.240	88	586	0.325	ng/ul	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042616.D
Acq On : 07 Nov 2023 17:30
Operator : MA/JU
Sample : 05026-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH328


Quant Time: Nov 07 23:06:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

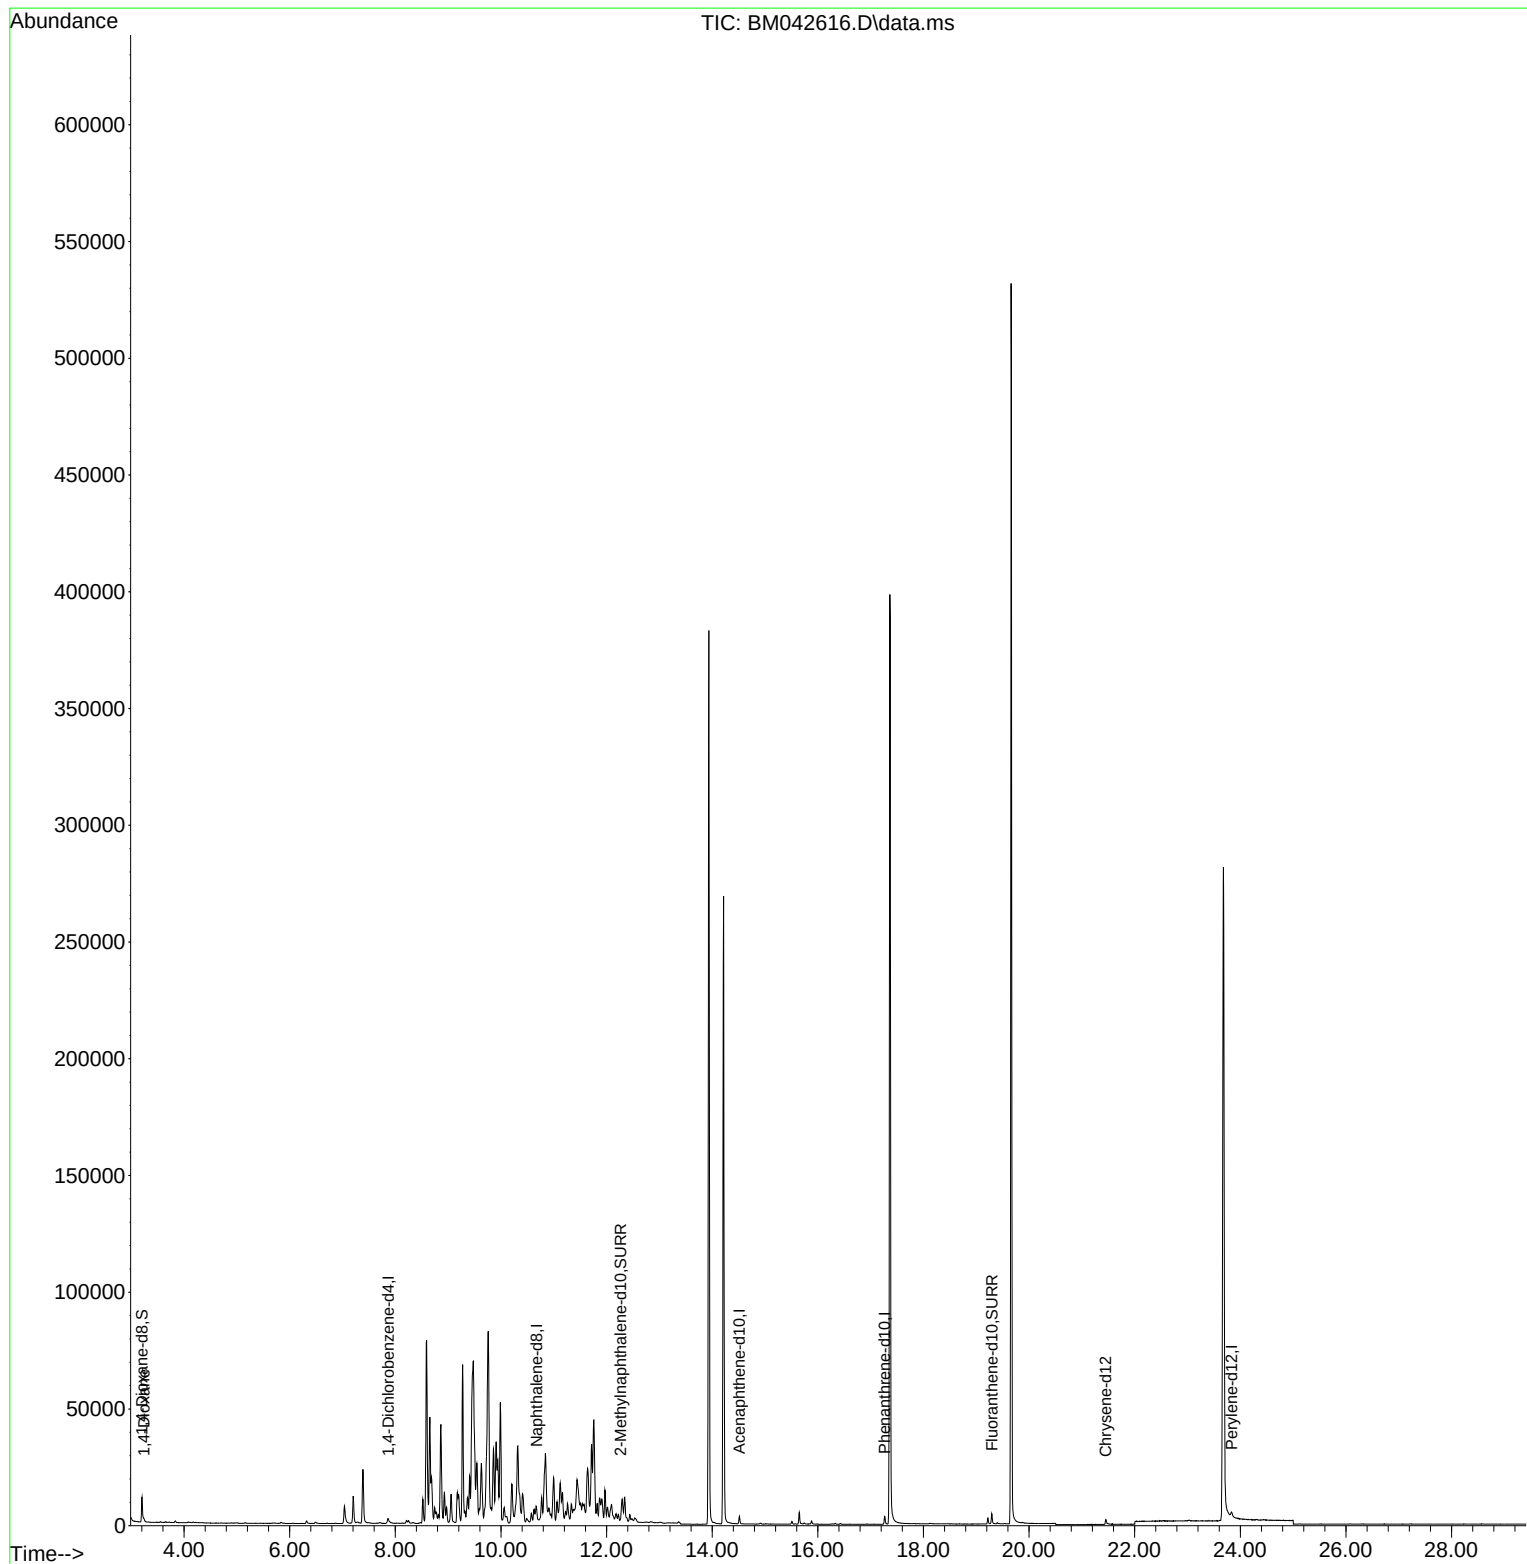

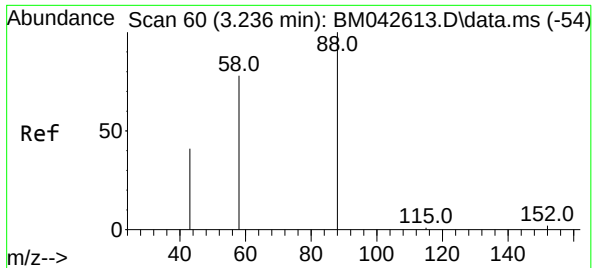

#2
 1,4-Dioxane
 Concen: 0.325 ng/ul
 RT: 3.240 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BM042616.D
 Acq: 07 Nov 2023 17:30

Instrument :
 BNA_M
 ClientSampleId :
 BH328

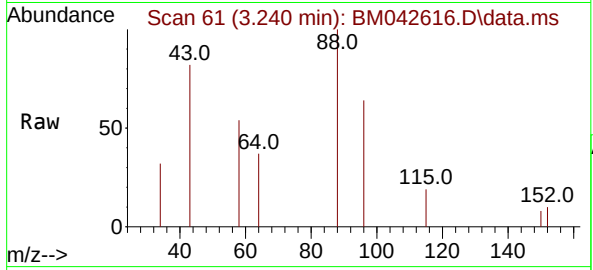

Tgt Ion: 88	Resp: 586
Ion Ratio	Lower Upper
88 100	
43 82.3	77.5 116.3
58 54.5	40.9 61.3

