

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042617.D
 Acq On : 07 Nov 2023 18:07
 Operator : MA/JU
 Sample : 05026-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH337

Quant Time: Nov 07 23:06:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1481	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.673	136	3568	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.516	164	2070	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.268	188	4715	0.400	ng/ul	0.00
17) Chrysene-d12	21.452	240	2843	0.400	ng/ul	0.00
23) Perylene-d12	23.832	264	3422	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	6666	3.406	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.267	152	1929	0.387	ng/ul	0.00
18) Fluoranthene-d10	19.295	212	4949	0.503	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.240	88	3389	1.457	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042617.D
Acq On : 07 Nov 2023 18:07
Operator : MA/JU
Sample : 05026-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH337


Quant Time: Nov 07 23:06:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

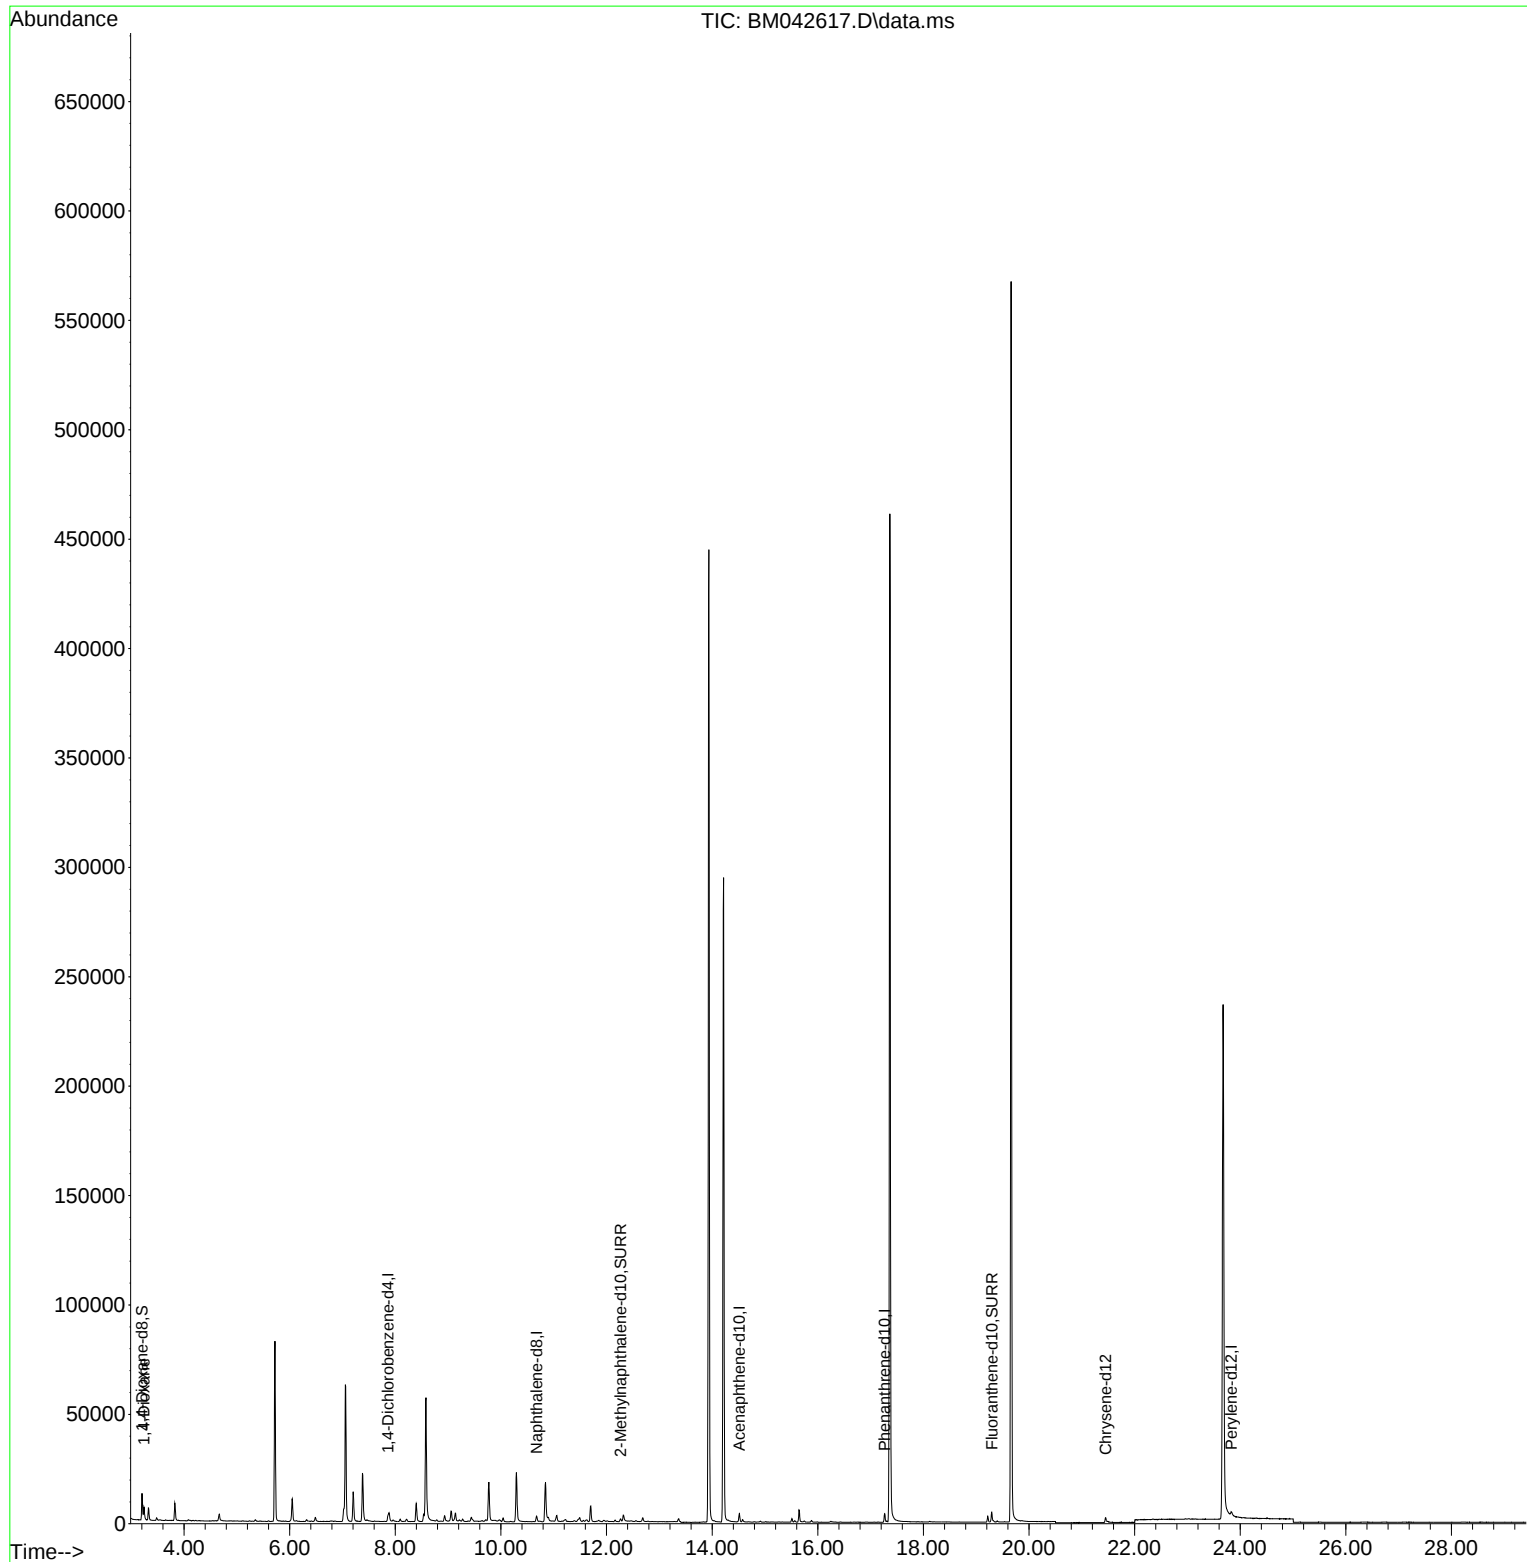

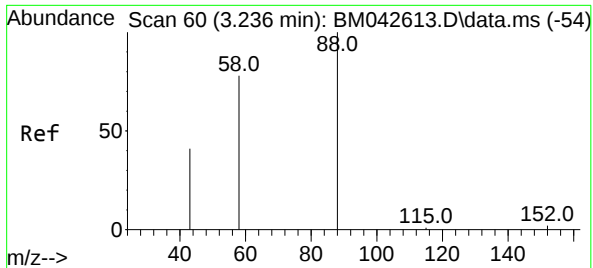

#2
 1,4-Dioxane
 Concen: 1.457 ng/ul
 RT: 3.240 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BM042617.D
 Acq: 07 Nov 2023 18:07

Instrument :
 BNA_M
 ClientSampleId :
 BH337

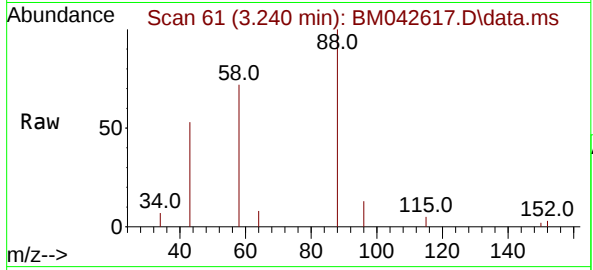

Tgt Ion: 88 Resp: 3389

Ion	Ratio	Lower	Upper
88	100		
43	53.5	77.5	116.3#
58	71.9	40.9	61.3#

