

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042619.D
 Acq On : 07 Nov 2023 19:19
 Operator : MA/JU
 Sample : 05026-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH340

Quant Time: Nov 07 23:06:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1277	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.678	136	2856	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.511	164	1784	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.264	188	4161	0.400	ng/ul	0.00
17) Chrysene-d12	21.450	240	2843	0.400	ng/ul	0.00
23) Perylene-d12	23.829	264	3797	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	5321	3.153	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.267	152	891	0.224	ng/ul	0.00
18) Fluoranthene-d10	19.290	212	2712	0.276	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.240	88	791	0.394	ng/ul	95




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042619.D
Acq On : 07 Nov 2023 19:19
Operator : MA/JU
Sample : 05026-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH340

Quant Time: Nov 07 23:06:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

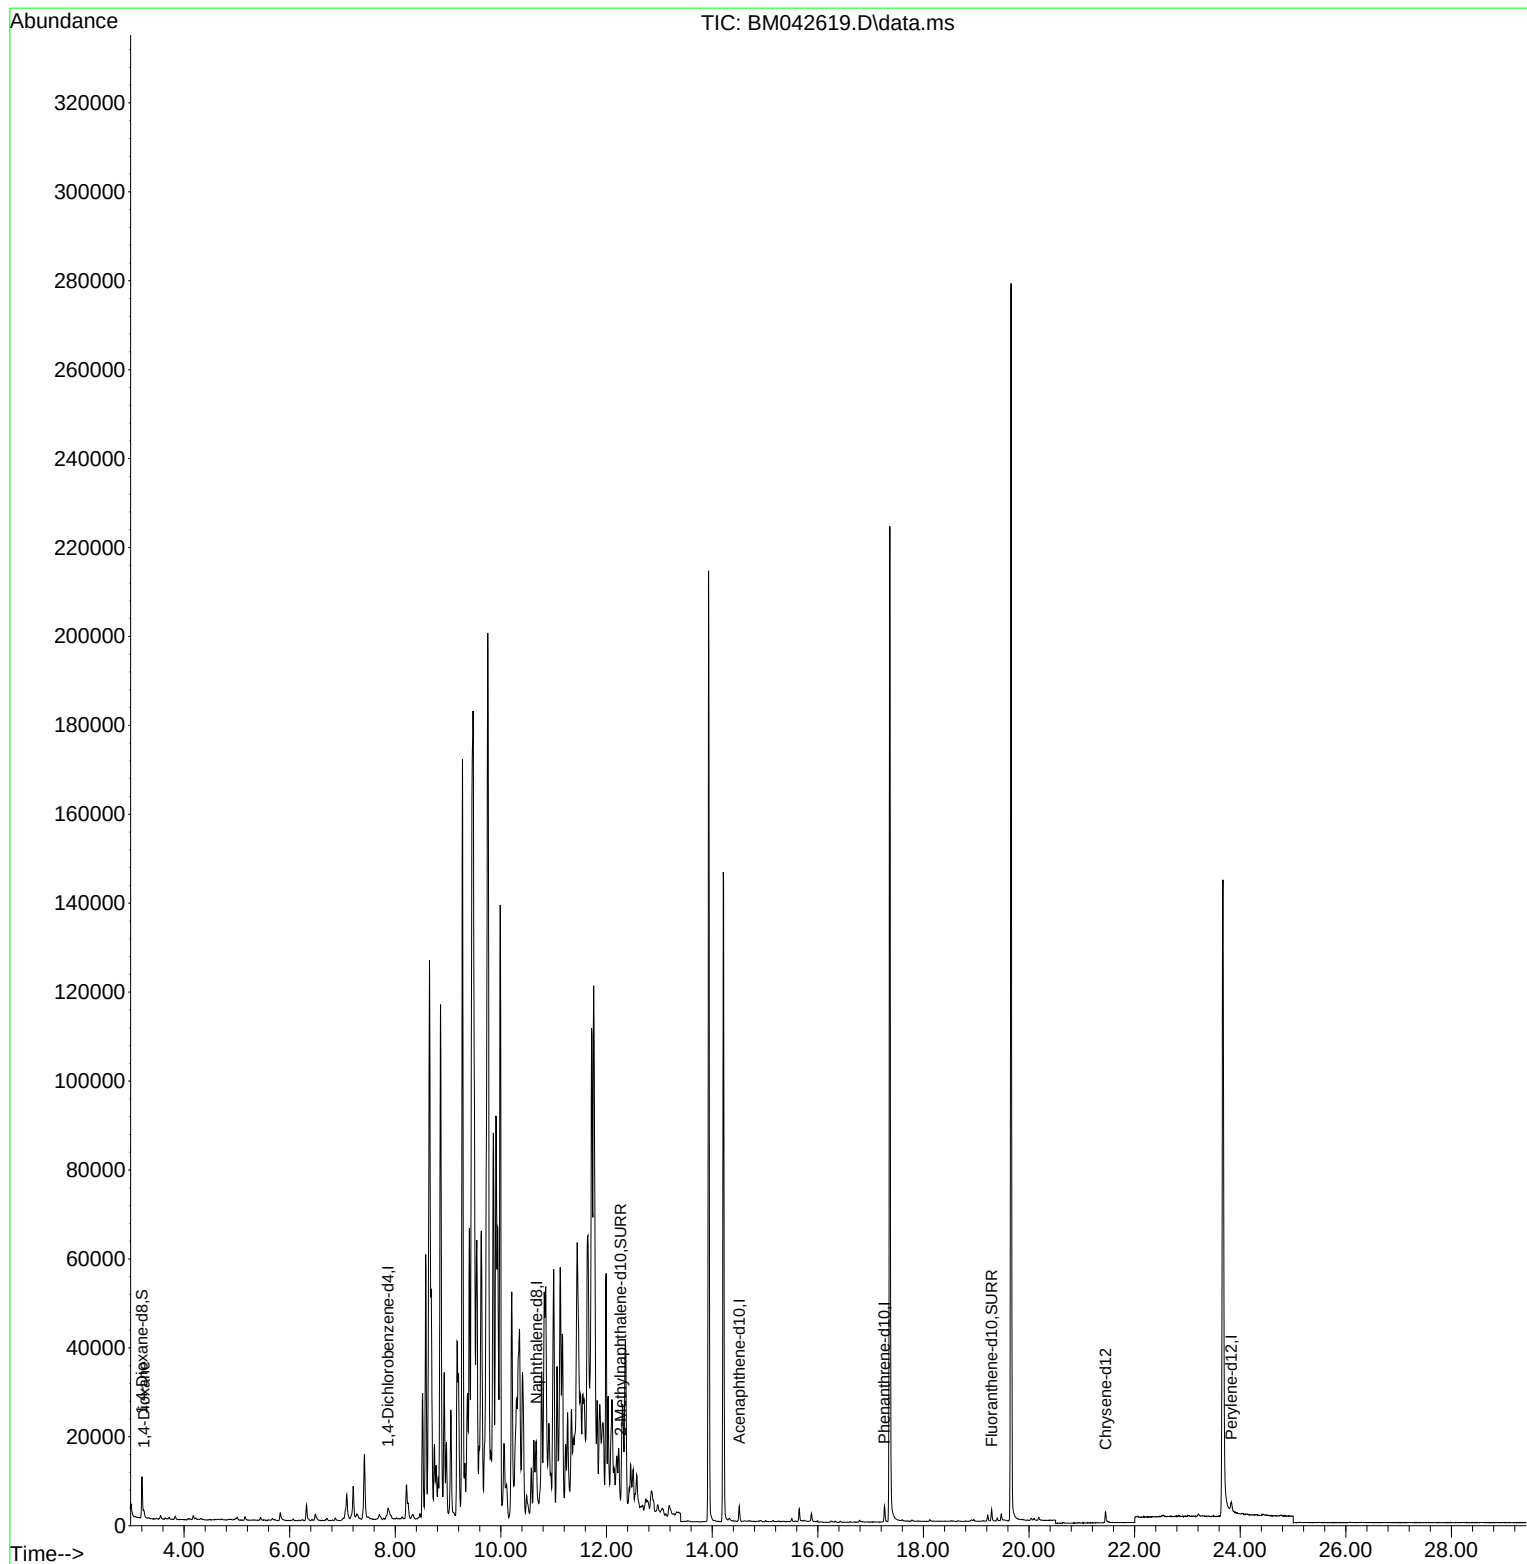

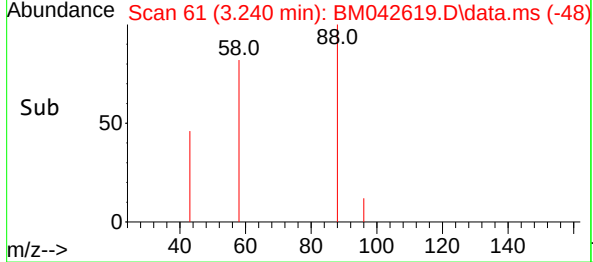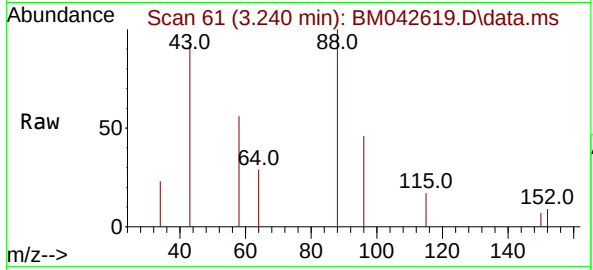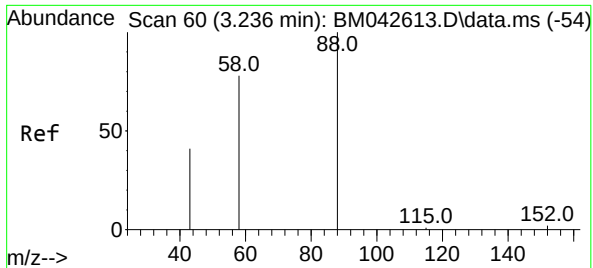

#2
 1,4-Dioxane
 Concen: 0.394 ng/ul
 RT: 3.240 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BM042619.D
 Acq: 07 Nov 2023 19:19

Ion	Ratio	Lower	Upper
88	100		
43	92.3	77.5	116.3
58	55.8	40.9	61.3

Instrument :
 BNA_M
 ClientSampleId :
 BH340

