

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042623.D
 Acq On : 07 Nov 2023 21:44
 Operator : MA/JU
 Sample : 05026-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH359

Quant Time: Nov 07 23:07:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.864	152	1047	0.400	ng/ul	0.00
4) Naphthalene-d8	10.671	136	2761	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.515	164	1669	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.267	188	3863	0.400	ng/ul	0.00
17) Chrysene-d12	21.450	240	2504	0.400	ng/ul	0.00
23) Perylene-d12	23.826	264	3558	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	6367	4.602	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.266	152	1564	0.406	ng/ul	0.00
18) Fluoranthene-d10	19.294	212	4534	0.523	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.240	88	393	0.239	ng/ul	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042623.D
Acq On : 07 Nov 2023 21:44
Operator : MA/JU
Sample : 05026-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH359

Quant Time: Nov 07 23:07:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

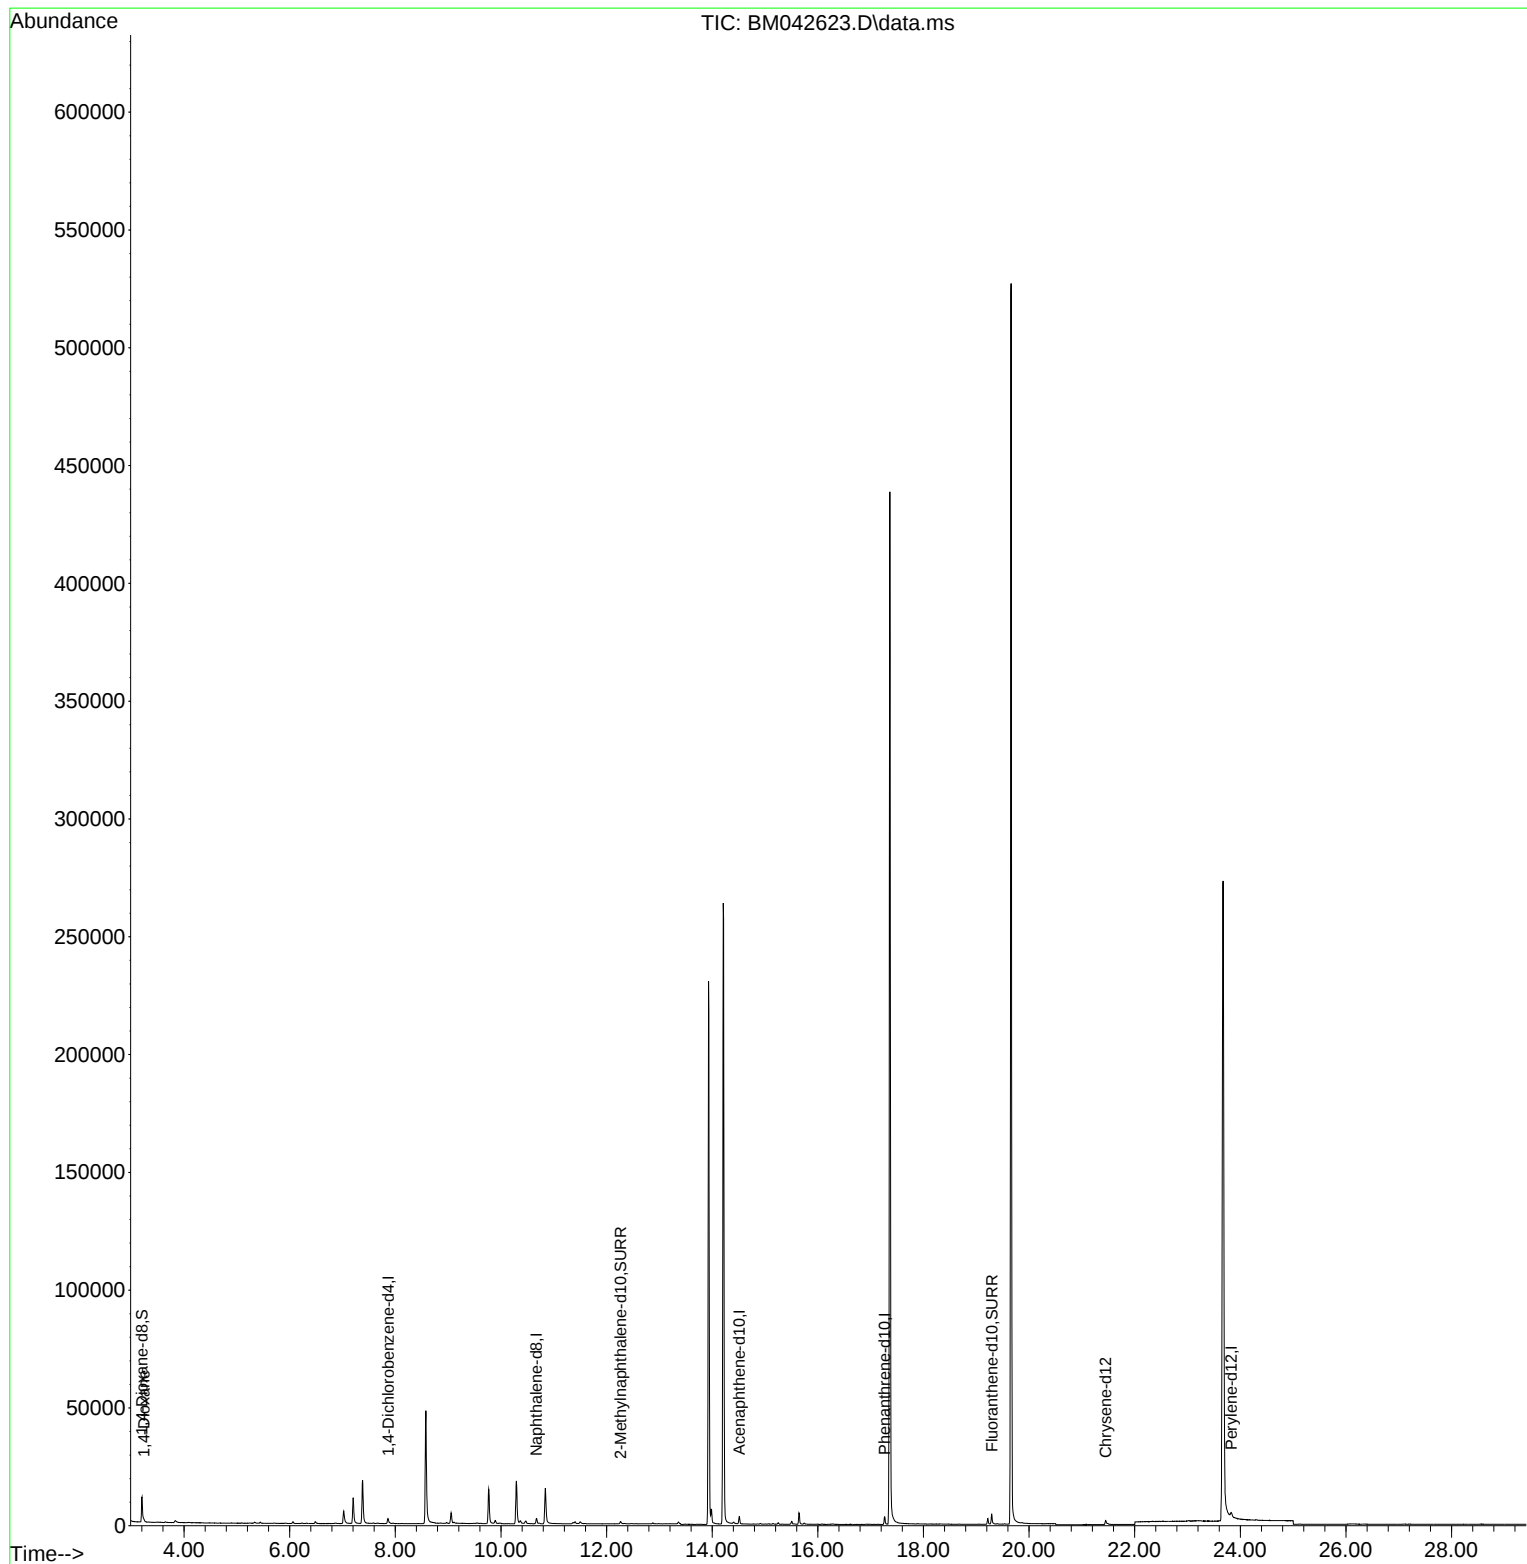

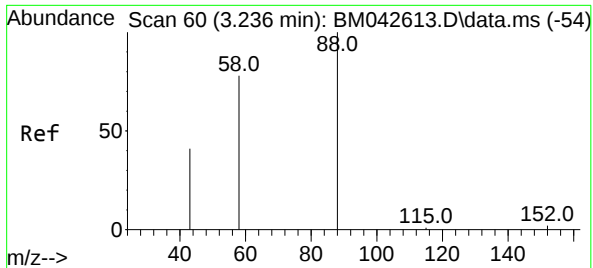

#2
 1,4-Dioxane
 Concen: 0.239 ng/ul
 RT: 3.240 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BM042623.D
 Acq: 07 Nov 2023 21:44

Instrument :
 BNA_M
 ClientSampleId :
 BH359

Tgt Ion:	88	Resp:	393
Ion	Ratio	Lower	Upper
88	100		
43	84.5	77.5	116.3
58	44.5	40.9	61.3

