

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042625.D
 Acq On : 07 Nov 2023 22:56
 Operator : MA/JU
 Sample : 05026-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH335

Quant Time: Nov 07 23:26:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1270	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.672	136	3204	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.511	164	1867	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.264	188	4443	0.400	ng/ul	0.00
17) Chrysene-d12	21.446	240	3060	0.400	ng/ul	0.00
23) Perylene-d12	23.826	264	4773	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	5782	3.445	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.262	152	1536	0.344	ng/ul	-0.01
18) Fluoranthene-d10	19.290	212	4427	0.418	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.239	88	656	0.329	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042625.D
Acq On : 07 Nov 2023 22:56
Operator : MA/JU
Sample : 05026-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH335


Quant Time: Nov 07 23:26:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

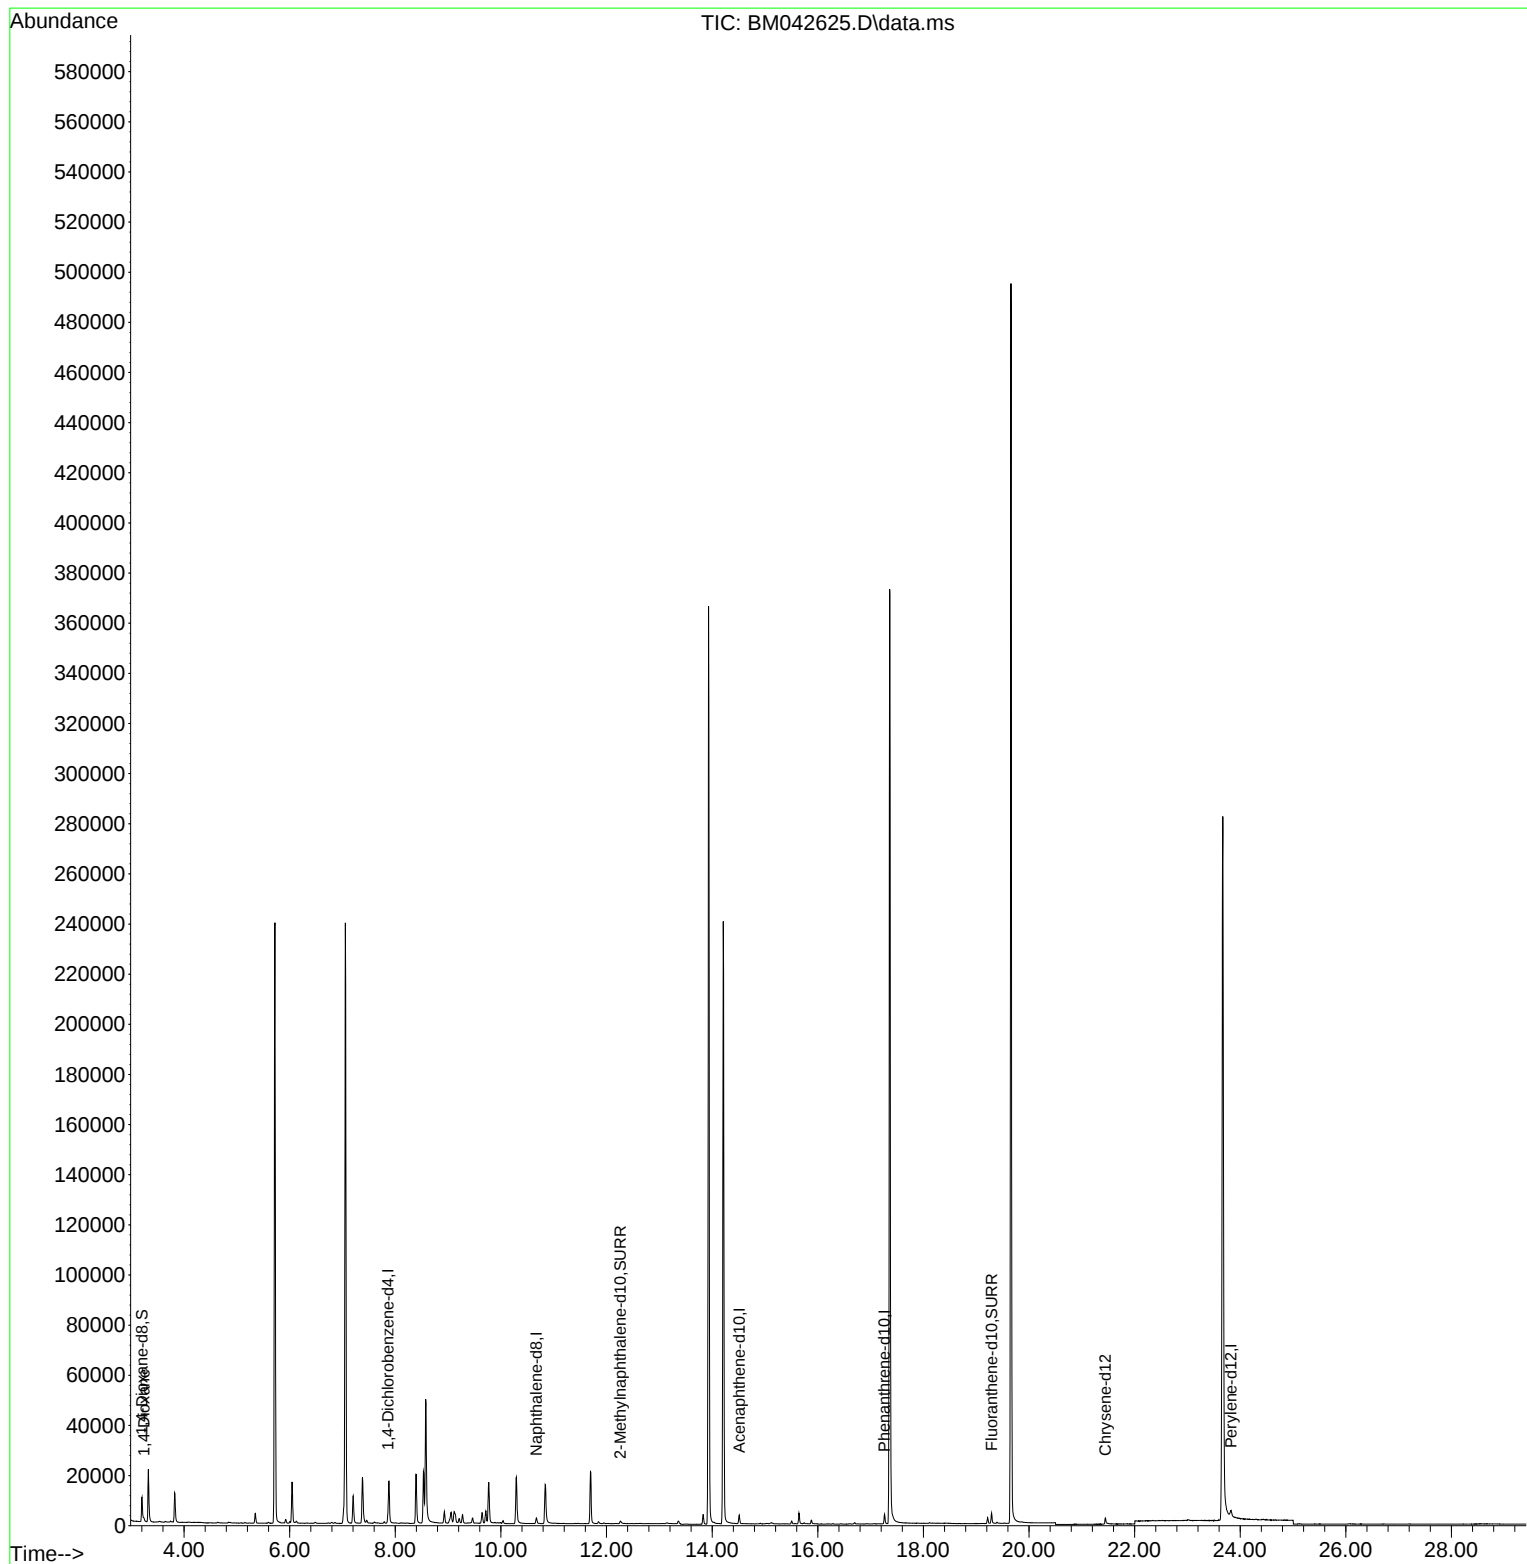

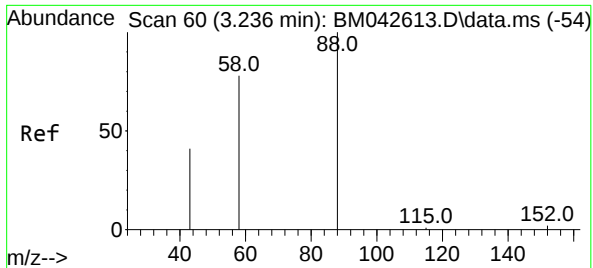

#2
 1,4-Dioxane
 Concen: 0.329 ng/ul
 RT: 3.239 min Scan# 61
 Delta R.T. -0.007 min
 Lab File: BM042625.D
 Acq: 07 Nov 2023 22:56

Instrument :
 BNA_M
 ClientSampleId :
 BH335

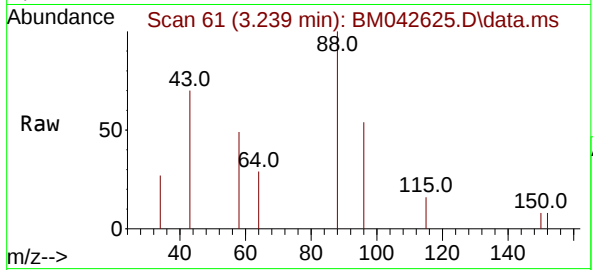

Tgt Ion: 88 Resp: 656
 Ion Ratio Lower Upper
 88 100
 43 70.0 77.5 116.3#
 58 48.5 40.9 61.3

