

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042626.D
 Acq On : 07 Nov 2023 23:32
 Operator : MA/JU
 Sample : 05026-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH338

Quant Time: Nov 08 00:16:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1508	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.673	136	3609	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.511	164	2113	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.264	188	4816	0.400	ng/ul	0.00
17) Chrysene-d12	21.450	240	3188	0.400	ng/ul	0.00
23) Perylene-d12	23.826	264	4508	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	7936	3.982	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.267	152	1939	0.385	ng/ul	0.00
18) Fluoranthene-d10	19.290	212	4772	0.432	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.240	88	1702	0.719	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042626.D
Acq On : 07 Nov 2023 23:32
Operator : MA/JU
Sample : 05026-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH338

Quant Time: Nov 08 00:16:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

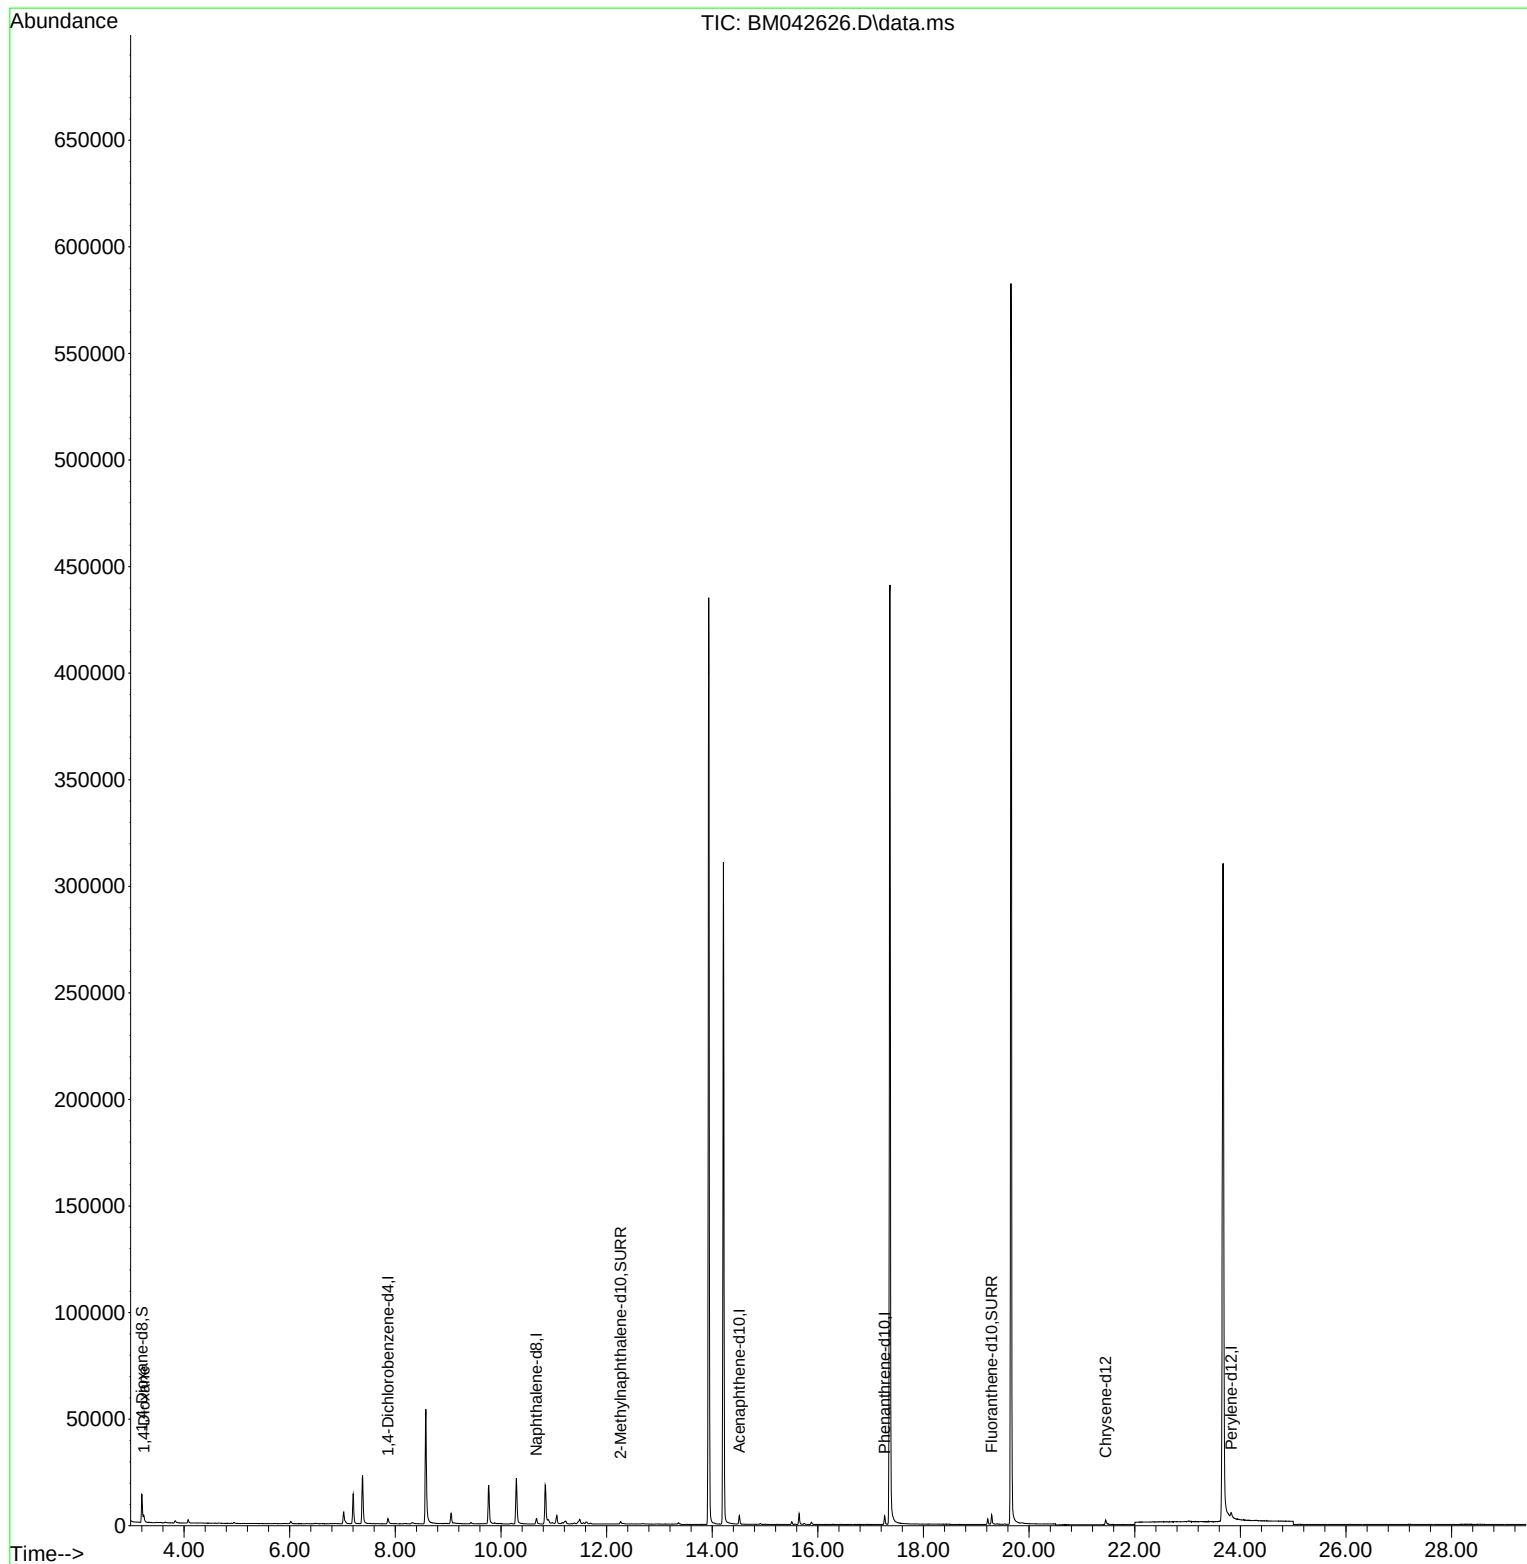

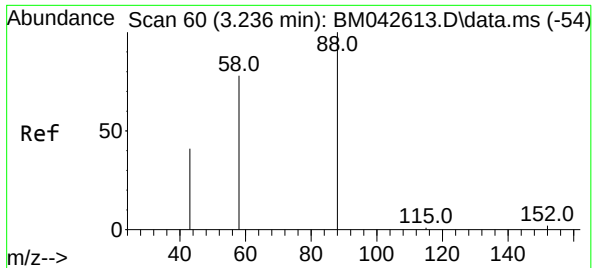

#2
 1,4-Dioxane
 Concen: 0.719 ng/ul
 RT: 3.240 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BM042626.D
 Acq: 07 Nov 2023 23:32

Instrument :
 BNA_M
 ClientSampleId :
 BH338

Tgt Ion: 88 Resp: 1702
 Ion Ratio Lower Upper
 88 100
 43 59.6 77.5 116.3#
 58 64.5 40.9 61.3#

