

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042627.D
 Acq On : 08 Nov 2023 00:08
 Operator : MA/JU
 Sample : 05026-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH336

Quant Time: Nov 08 00:54:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1396	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.673	136	3500	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.511	164	2031	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.264	188	4598	0.400	ng/ul	0.00
17) Chrysene-d12	21.447	240	3022	0.400	ng/ul	0.00
23) Perylene-d12	23.823	264	4046	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	6362	3.449	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.262	152	1651	0.338	ng/ul	-0.01
18) Fluoranthene-d10	19.290	212	4777	0.457	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.240	88	368	0.168	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042627.D
Acq On : 08 Nov 2023 00:08
Operator : MA/JU
Sample : 05026-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH336

Quant Time: Nov 08 00:54:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

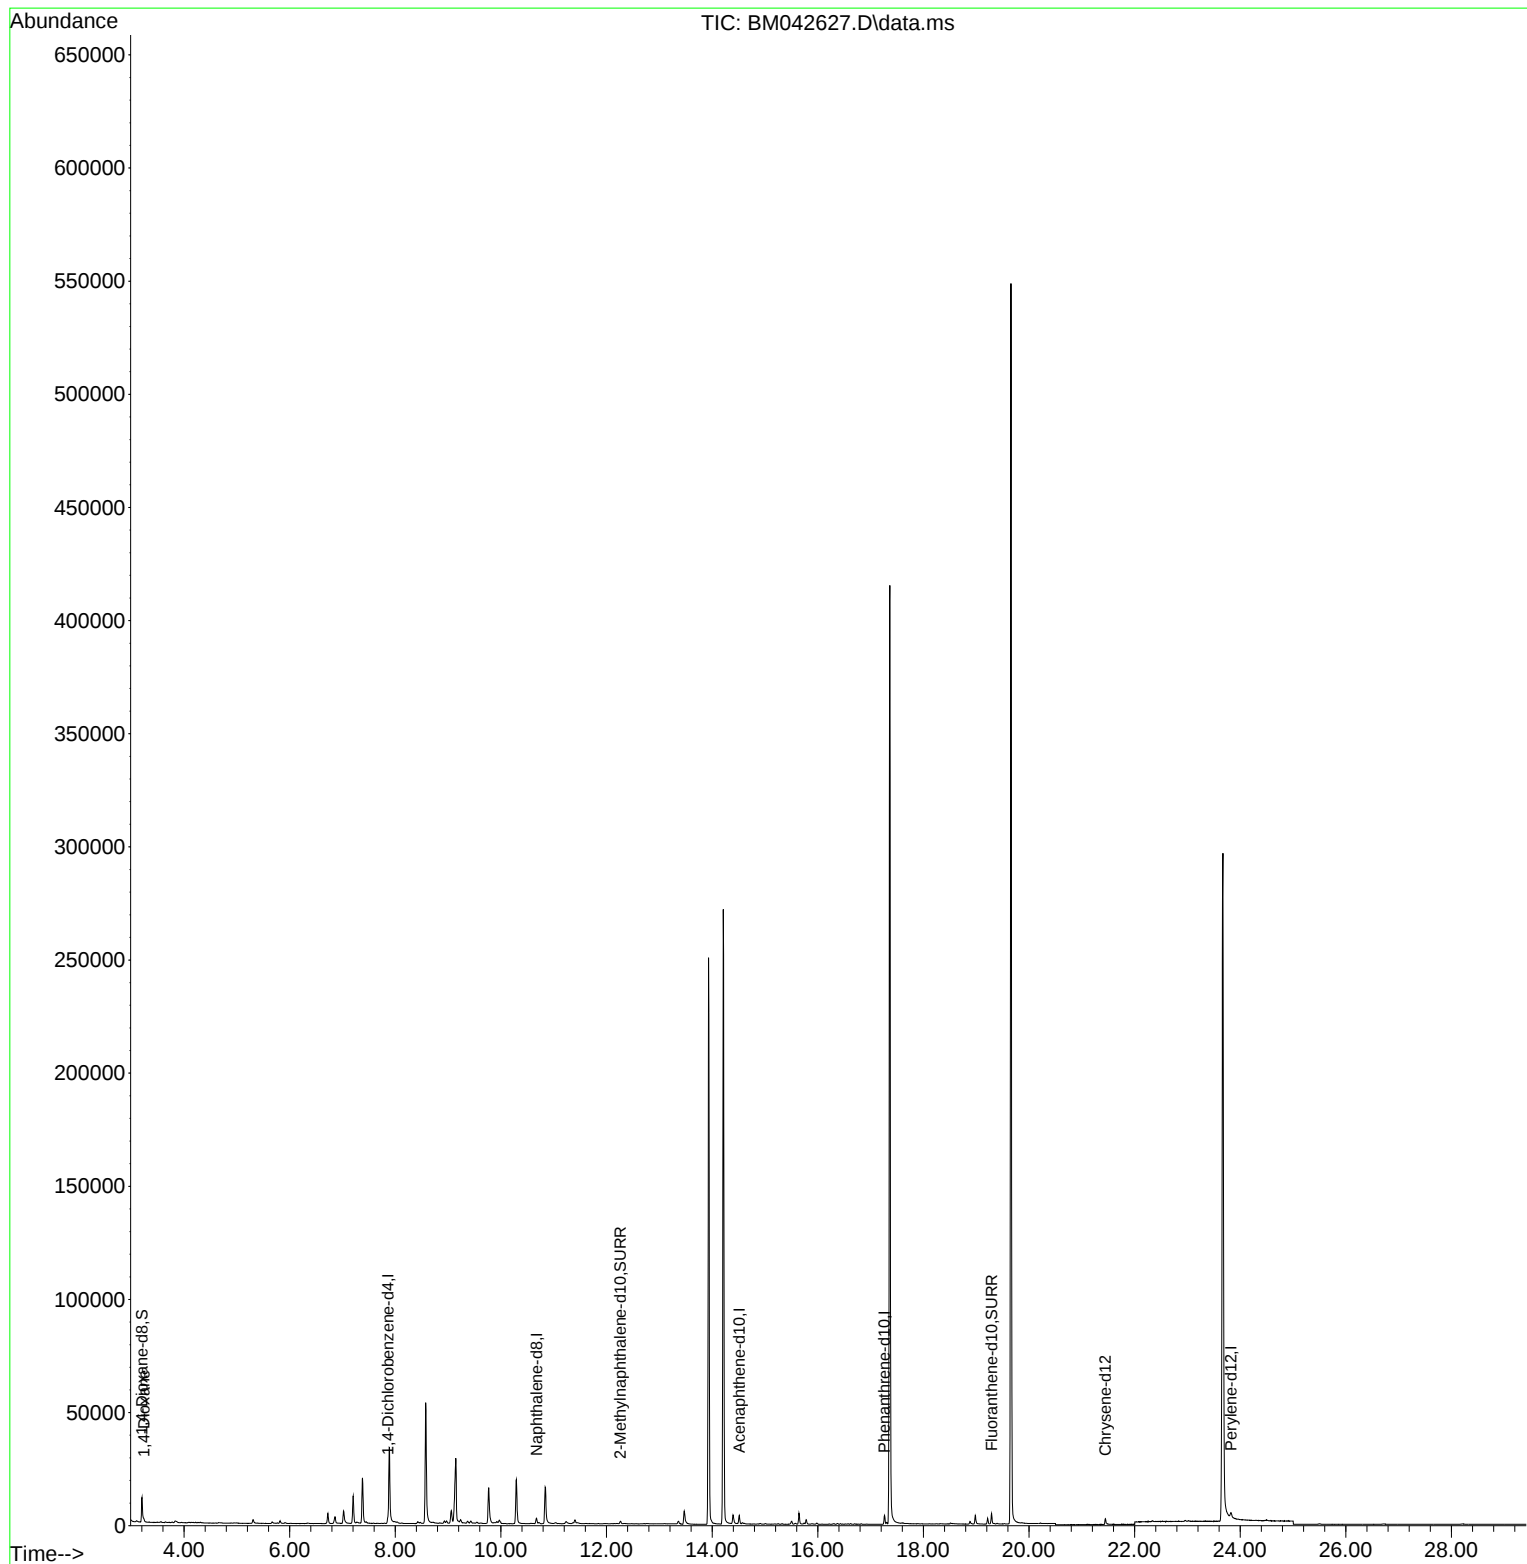

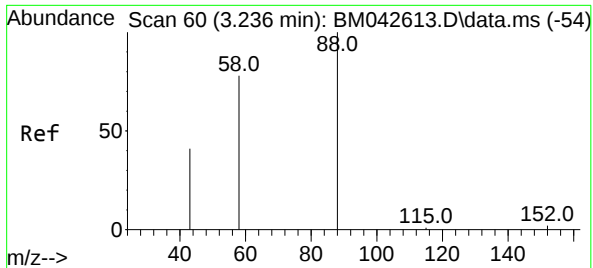

#2
 1,4-Dioxane
 Concen: 0.168 ng/ul
 RT: 3.240 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BM042627.D
 Acq: 08 Nov 2023 00:08

Instrument :
 BNA_M
 ClientSampleId :
 BH336

Tgt Ion: 88	Resp: 368
Ion Ratio	Lower Upper
88	100
43	130.1 77.5 116.3#
58	44.7 40.9 61.3

