

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042628.D
 Acq On : 08 Nov 2023 00:45
 Operator : MA/JU
 Sample : 05026-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH344

Quant Time: Nov 08 01:23:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.860	152	1199	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.673	136	3126	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.511	164	2130	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.264	188	4579	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.447	240	3011	0.400	ng/ul	0.00
23) Perylene-d12	23.823	264	4004	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	5624	3.549	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.262	152	1652	0.379	ng/ul	-0.01
18) Fluoranthene-d10	19.290	212	4841	0.464	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.236	88	10497	5.574	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042628.D
Acq On : 08 Nov 2023 00:45
Operator : MA/JU
Sample : 05026-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH344

Quant Time: Nov 08 01:23:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

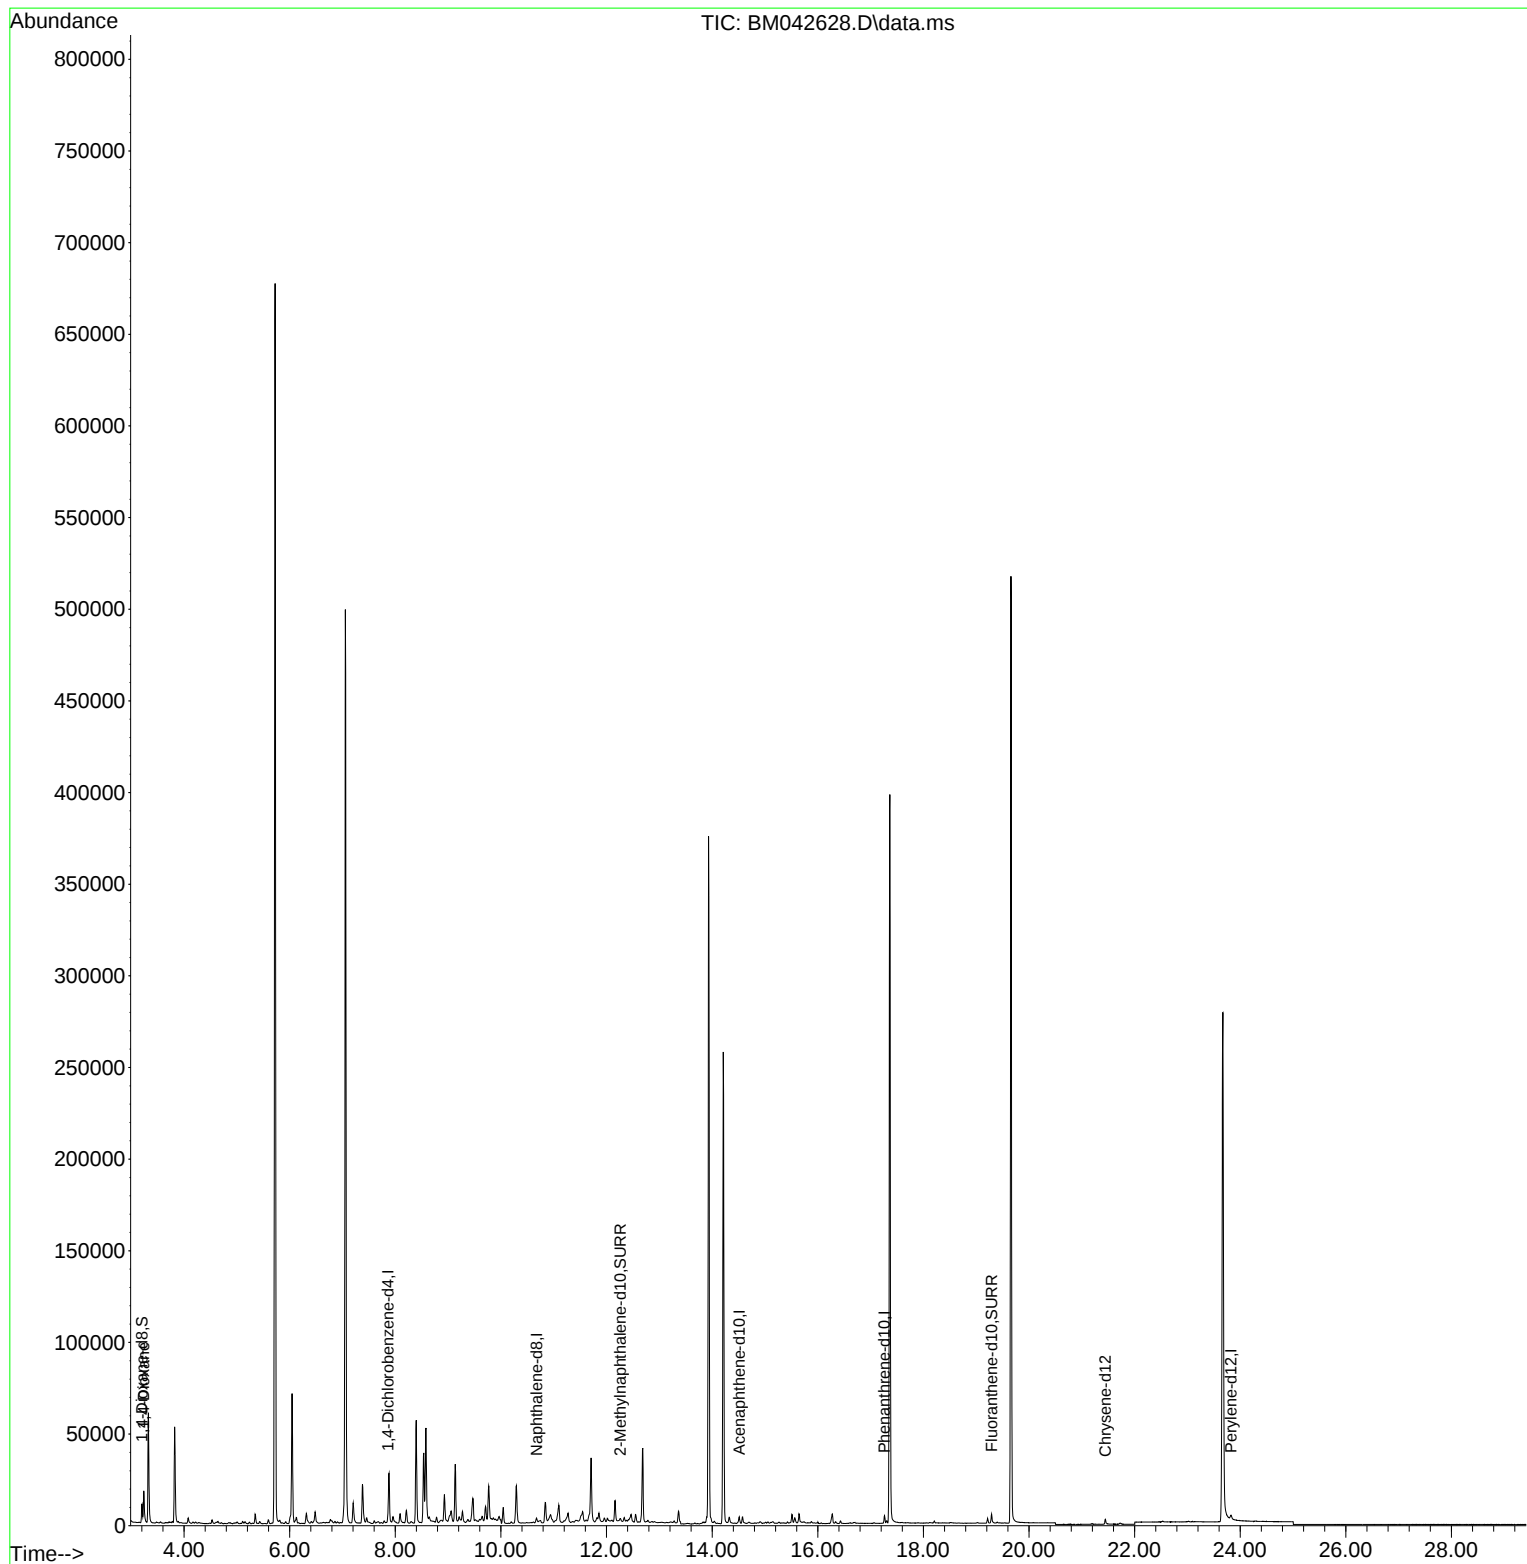

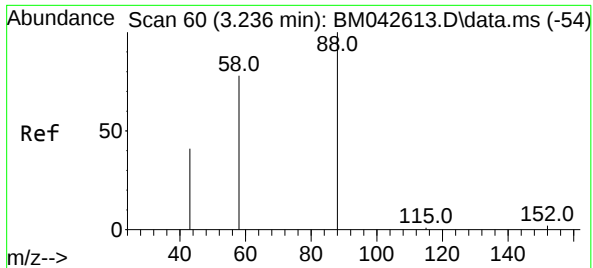

#2
 1,4-Dioxane
 Concen: 5.574 ng/ul
 RT: 3.236 min Scan# 60
 Delta R.T. -0.010 min
 Lab File: BM042628.D
 Acq: 08 Nov 2023 00:45

Instrument :
 BNA_M
 ClientSampleId :
 BH344

Tgt Ion: 88 Resp: 10497

Ion	Ratio	Lower	Upper
88	100		
43	51.3	77.5	116.3#
58	81.6	40.9	61.3#

