

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042635.D
 Acq On : 08 Nov 2023 05:33
 Operator : MA/JU
 Sample : 05026-16
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH326

Quant Time: Nov 08 06:02:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1523	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.671	136	3953	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.510	164	2210	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.262	188	5296	0.400	ng/ul	0.00
17) Chrysene-d12	21.447	240	3627	0.400	ng/ul	0.00
23) Perylene-d12	23.823	264	4881	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	7412	3.683	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.266	152	1916	0.347	ng/ul	0.00
18) Fluoranthene-d10	19.289	212	6036	0.481	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.240	88	379	0.158	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042635.D
Acq On : 08 Nov 2023 05:33
Operator : MA/JU
Sample : 05026-16
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH326

Quant Time: Nov 08 06:02:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

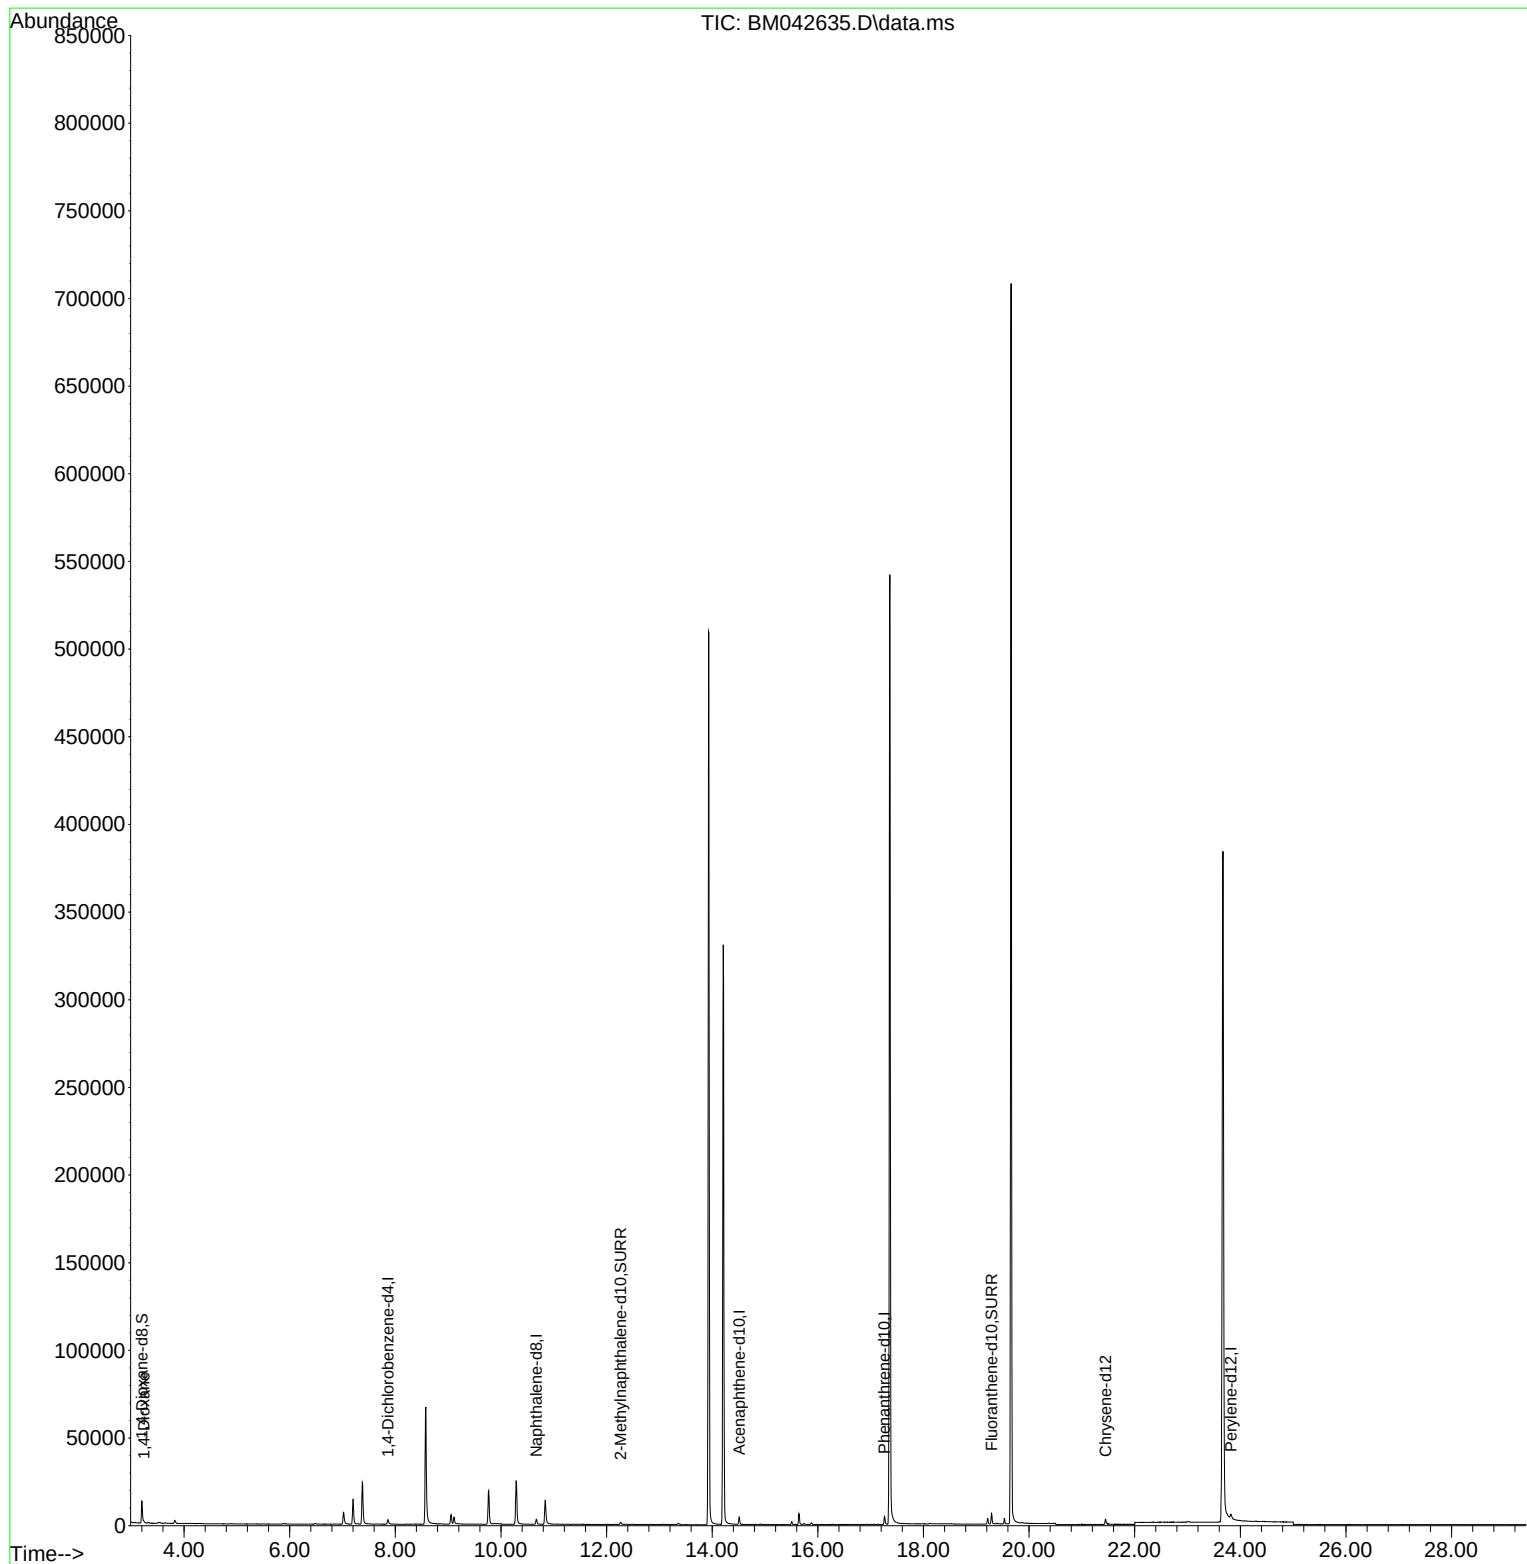

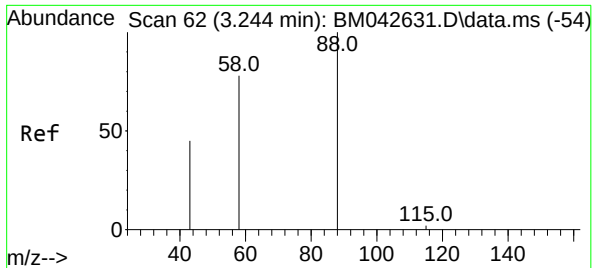

#2
 1,4-Dioxane
 Concen: 0.158 ng/ul
 RT: 3.240 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BM042635.D
 Acq: 08 Nov 2023 05:33

Instrument :
 BNA_M
 ClientSampleId :
 BH326

Tgt Ion:	88	Resp:	379
Ion	Ratio	Lower	Upper
88	100		
43	78.6	77.5	116.3
58	39.4	40.9	61.3#

