

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
 Data File : BM042638.D
 Acq On : 08 Nov 2023 07:21
 Operator : MA/JU
 Sample : 05026-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH346

Quant Time: Nov 08 07:50:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 07 02:23:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.859	152	1215	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.671	136	2983	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.510	164	1717	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.262	188	3913	0.400	ng/ul	0.00
17) Chrysene-d12	21.453	240	2605	0.400	ng/ul	0.00
23) Perylene-d12	23.826	264	3629	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.202	96	5805	3.615	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.266	152	1474	0.354	ng/ul	0.00
18) Fluoranthene-d10	19.289	212	4005	0.444	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.235	88	2197	1.151	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110723\
Data File : BM042638.D
Acq On : 08 Nov 2023 07:21
Operator : MA/JU
Sample : 05026-19
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH346

Quant Time: Nov 08 07:50:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 07 02:23:03 2023
Response via : Initial Calibration

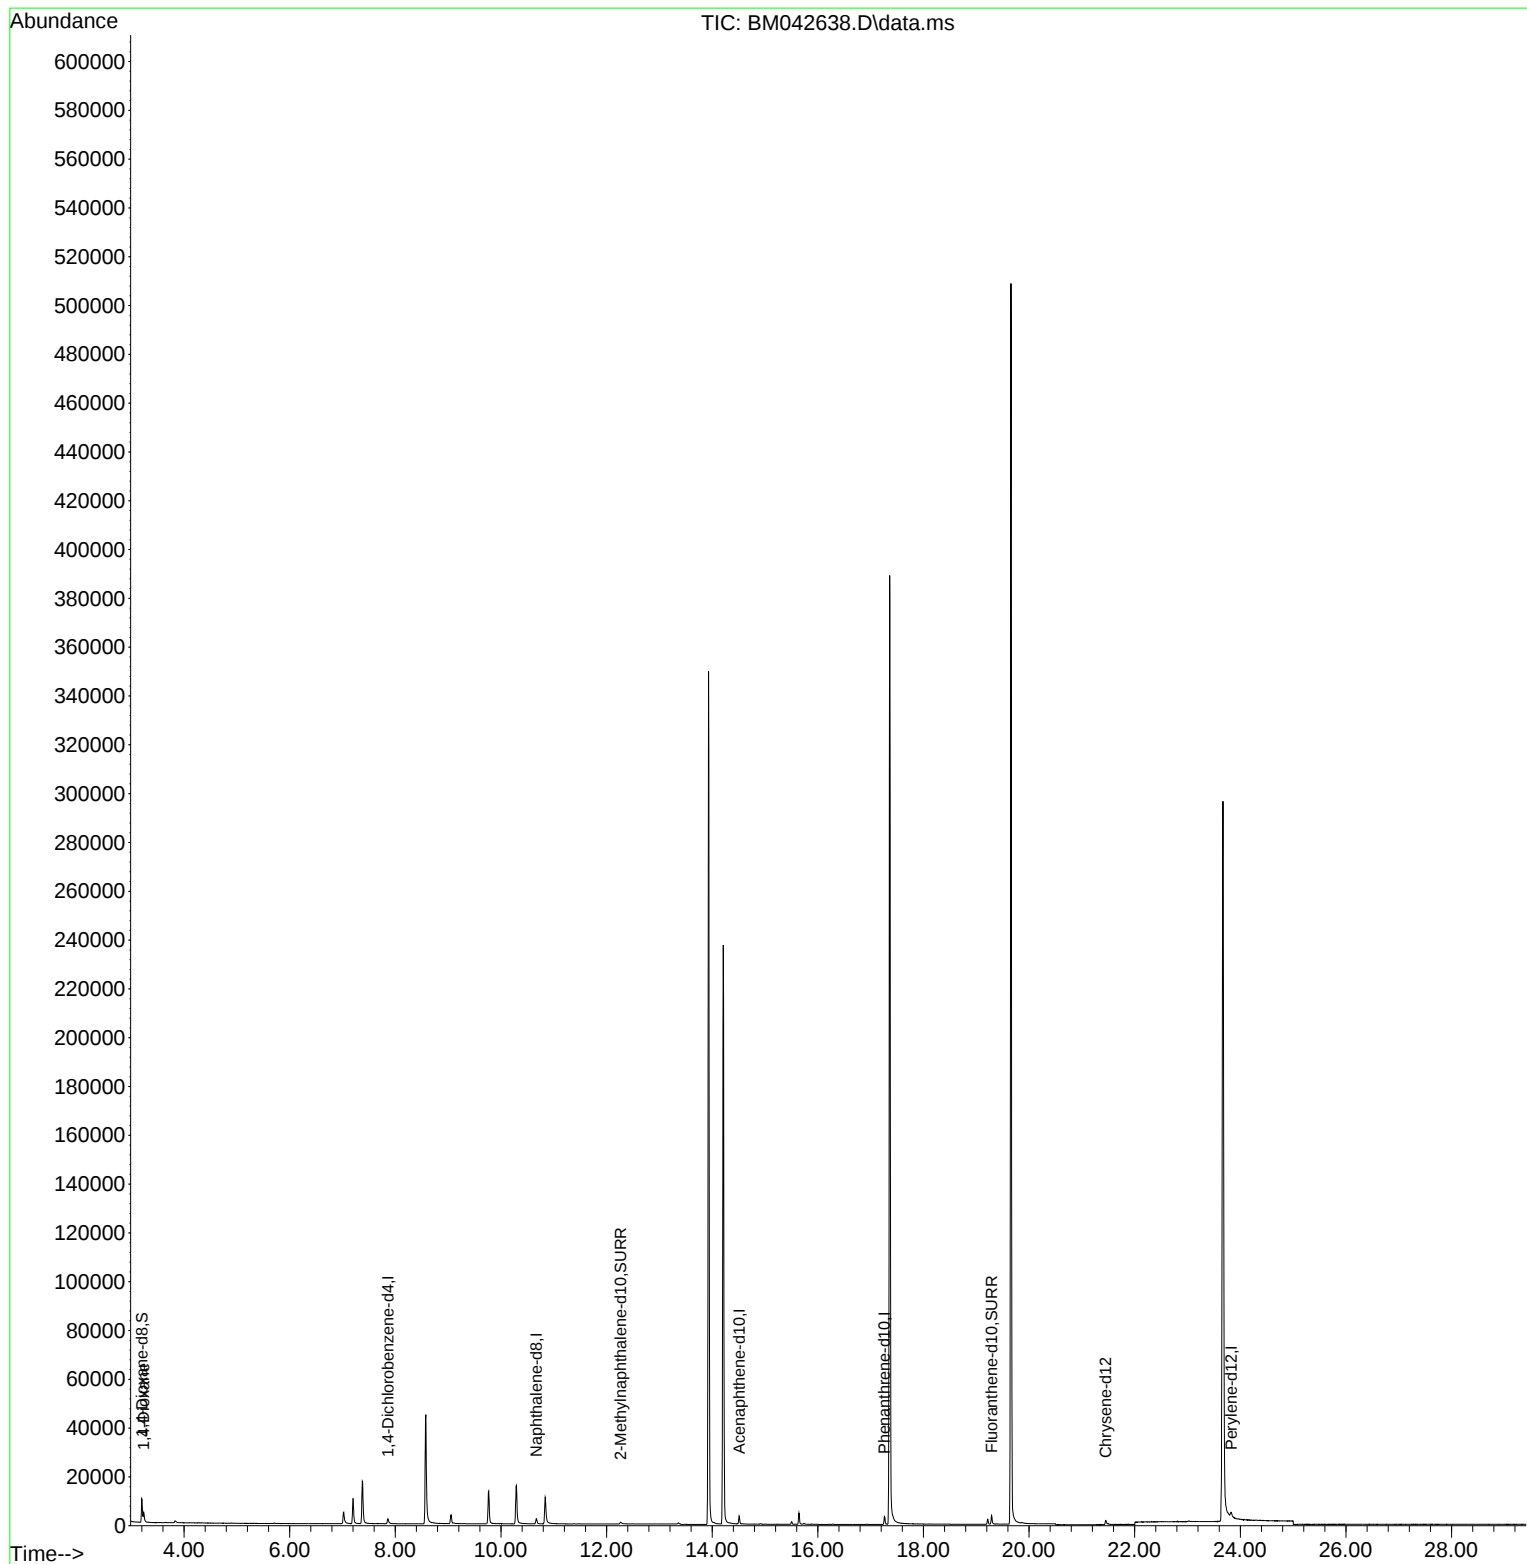

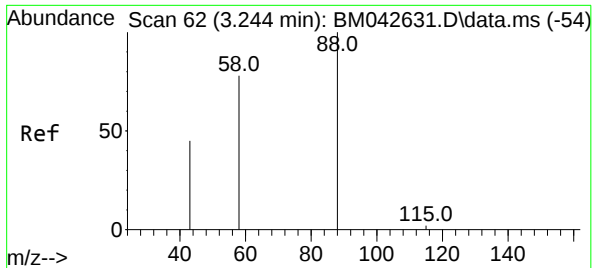

#2
 1,4-Dioxane
 Concen: 1.151 ng/ul
 RT: 3.235 min Scan# 60
 Delta R.T. -0.011 min
 Lab File: BM042638.D
 Acq: 08 Nov 2023 07:21

Instrument :
 BNA_M
 ClientSampleId :
 BH346

Tgt Ion: 88 Resp: 2197

Ion	Ratio	Lower	Upper
88	100		
43	55.3	77.5	116.3#
58	69.3	40.9	61.3#

