


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM110818\
 Data File : BM017550.D
 Acq On : 07 Nov 2018 08:55
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 15:08:36 2018

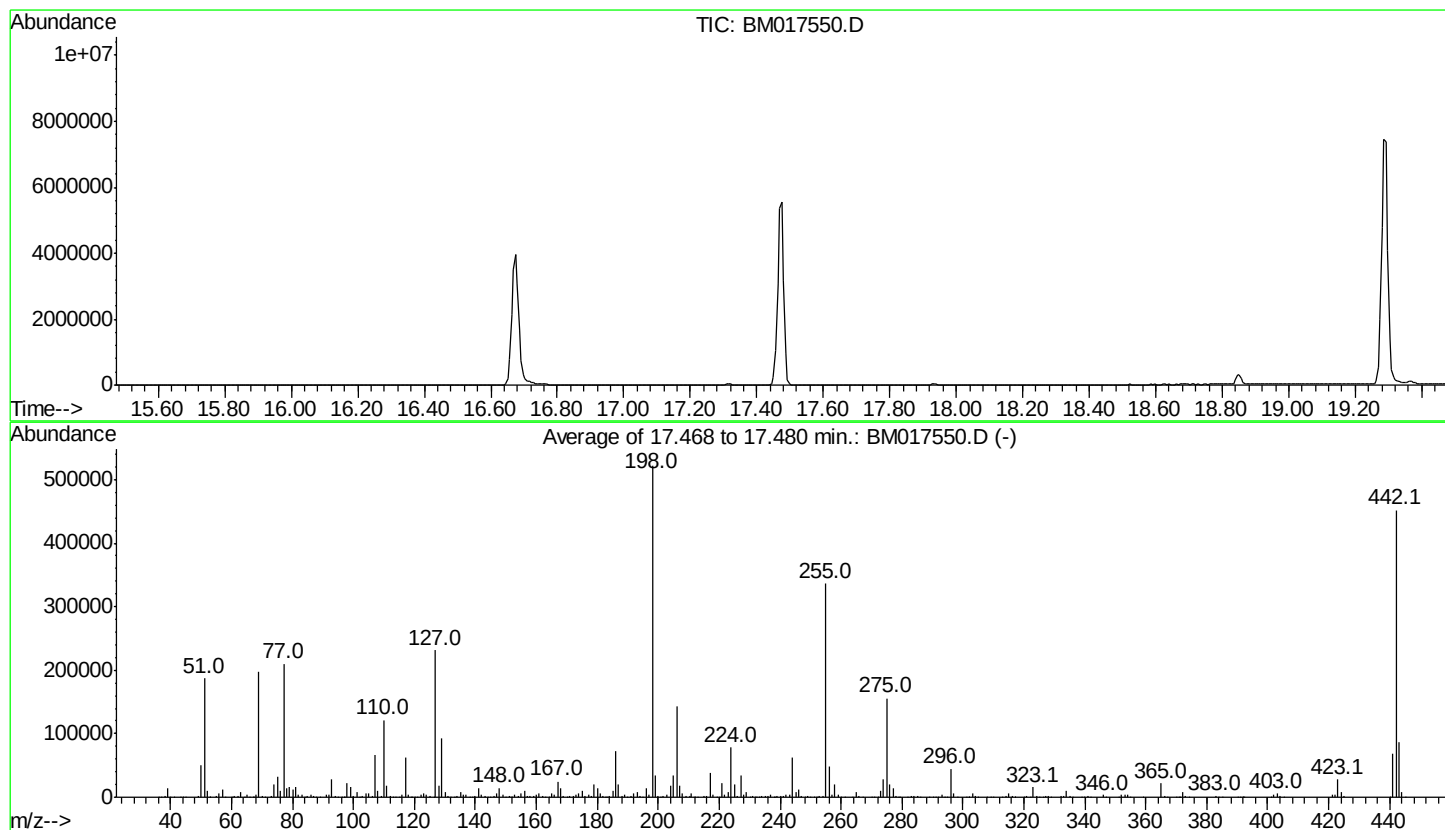

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	187008	PASS
68	69	0.00	2	1.9	3746	PASS
69	198	0.00	100	38.0	198154	PASS
70	69	0.00	2	0.6	1113	PASS
127	198	10	80	44.3	231274	PASS
197	198	0.00	2	0.6	3326	PASS
198	198	100	100	100.0	521984	PASS
199	198	5	9	6.7	34906	PASS
275	198	10	60	29.8	155696	PASS
365	198	1	100	4.2	21690	PASS
441	198	0.01	100	13.1	68562	PASS
442	198	50	100	86.6	452117	PASS
443	442	15	24	19.1	86384	PASS