
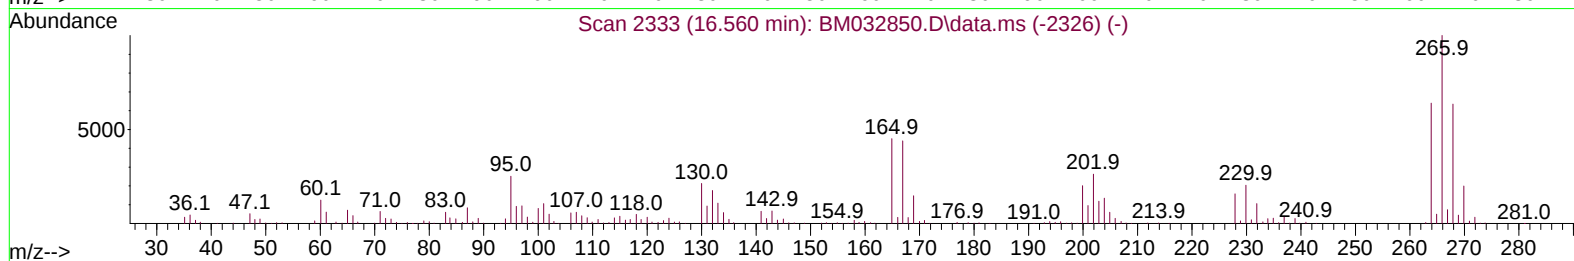
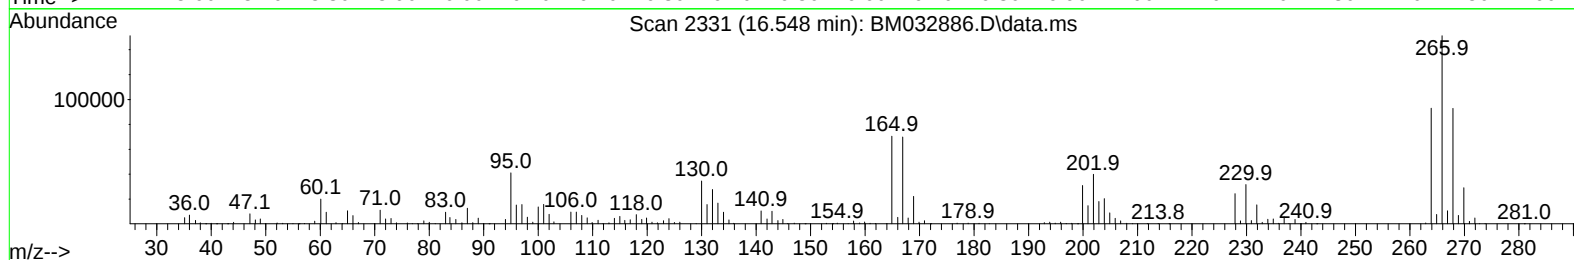


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110821\
Data File : BM032886.D
Acq On : 08 Nov 2021 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 11:17:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 16:07:18 2021
Response via : Initial Calibration

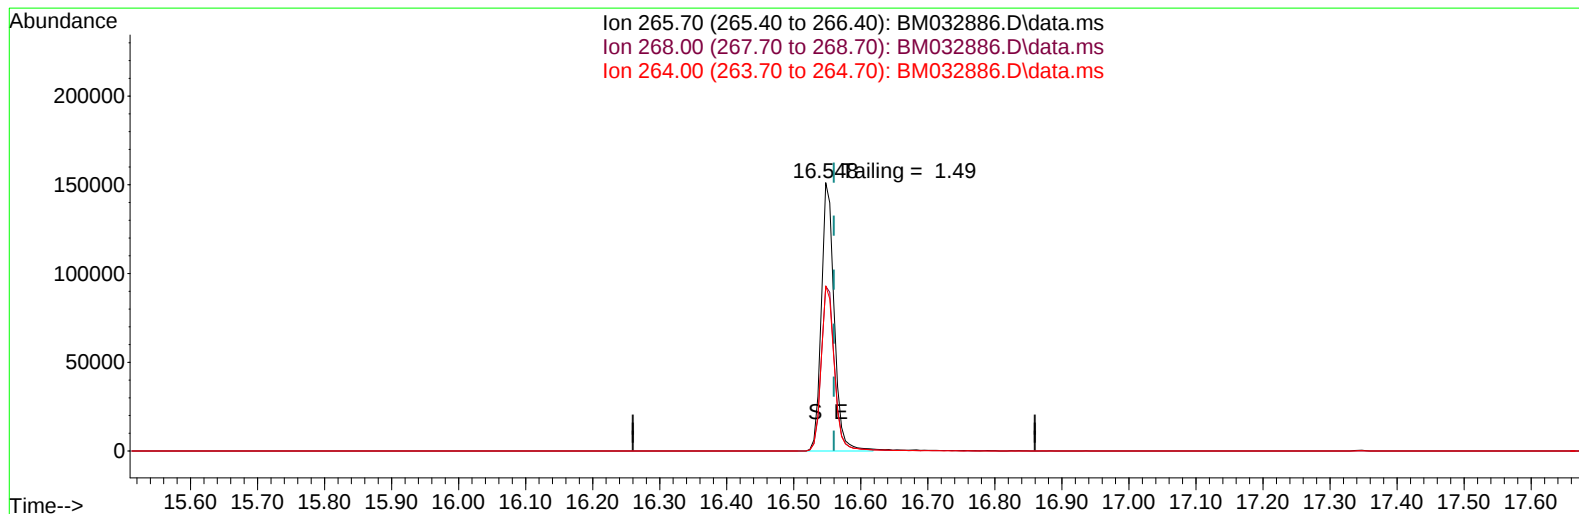

TIC: BM032886.D\data.ms

(70) Pentachlorophenol (C)




16.548min (-0.012) 0.00 ng

response 204349

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	61.41
264.00	65.10	61.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110821\
Data File : BM032886.D
Acq On : 08 Nov 2021 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 08 11:17:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 16:07:18 2021
Response via : Initial Calibration

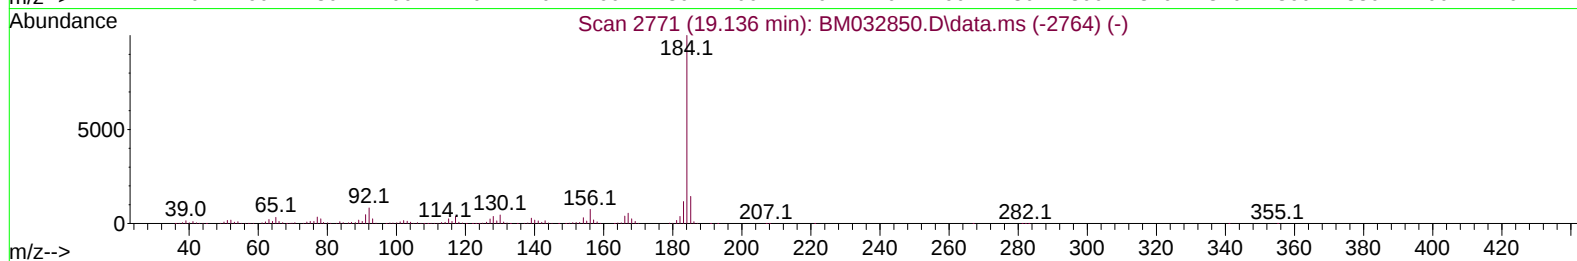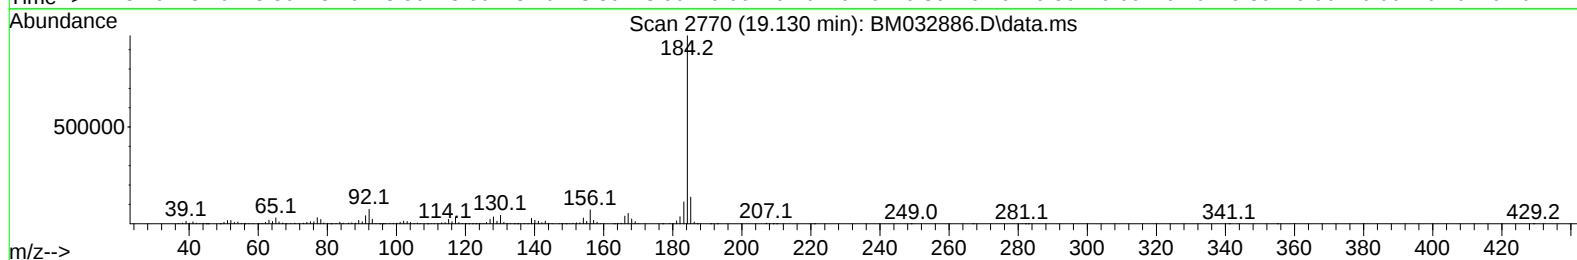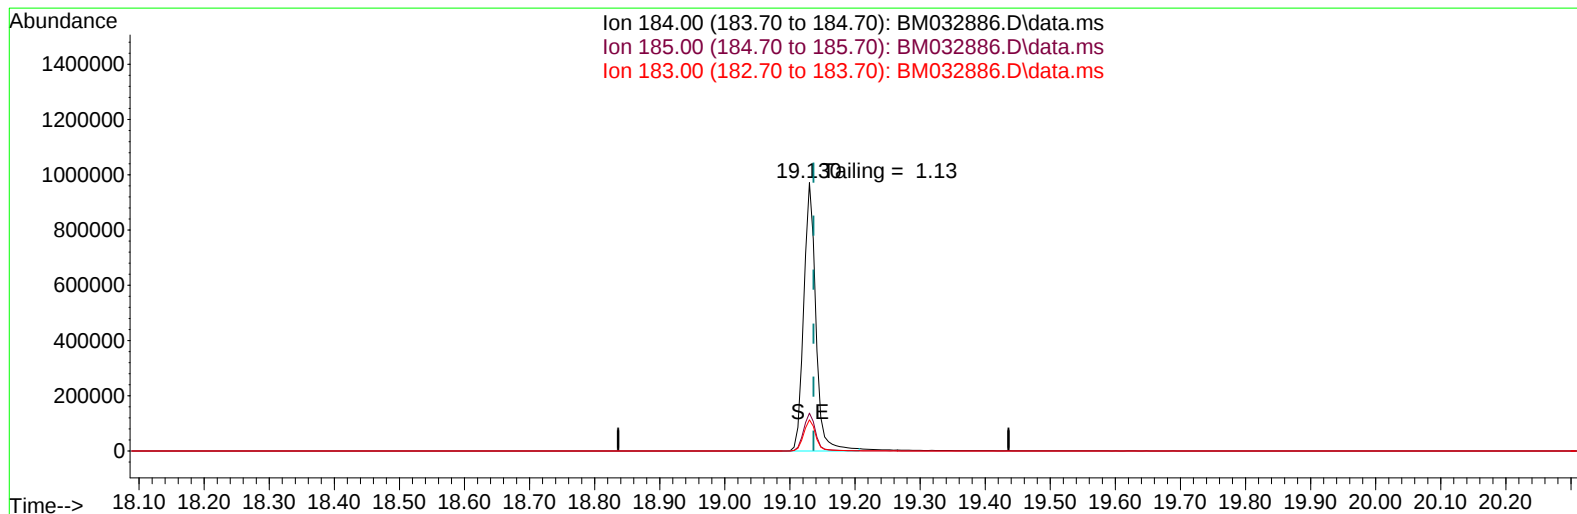

TIC: BM032886.D\data.ms

(77) Benzidine

19.130min (-0.006) 0.00 ng

response 1282605

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.15
183.00	11.20	11.66
0.00	0.00	0.00