

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110821\
 Data File : BM032888.D
 Acq On : 08 Nov 2021 10:59
 Operator : CG/JU
 Sample : PB140521BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB140521BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.078	374	381	407	rBV	2713236	3784114	45.59%	10.247%
2	6.695	648	656	668	rBV	2403605	3884100	46.79%	10.517%
3	7.484	783	790	808	rBV	427662	676596	8.15%	1.832%
4	8.636	979	986	1007	rBV	1564319	2514664	30.29%	6.809%
5	10.266	1255	1263	1278	rBV	598600	968704	11.67%	2.623%
6	12.760	1680	1687	1708	rBV	3801249	5793055	69.79%	15.686%
7	14.142	1916	1922	1940	rBV	939611	1374149	16.55%	3.721%
8	15.642	2170	2177	2202	rBV	2946722	4479889	53.97%	12.131%
9	16.883	2382	2388	2400	rBV	1211271	1687008	20.32%	4.568%
10	19.518	2829	2836	2847	rBV	6174186	8300828	100.00%	22.477%
11	21.065	3094	3099	3110	rBV	1457155	1818281	21.90%	4.923%
12	23.177	3452	3458	3468	rBV2	941469	1649391	19.87%	4.466%




Sum of corrected areas: 36930779

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110821\
Data File : BM032888.D
Acq On : 08 Nov 2021 10:59
Operator : CG/JU
Sample : PB140521BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140521BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

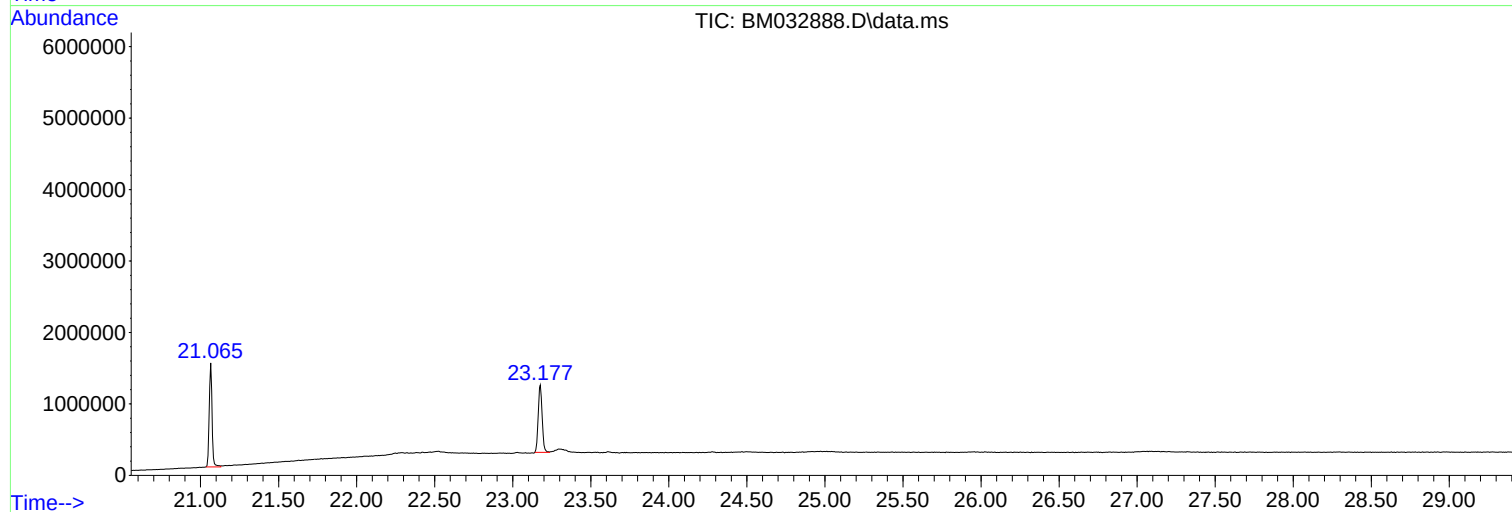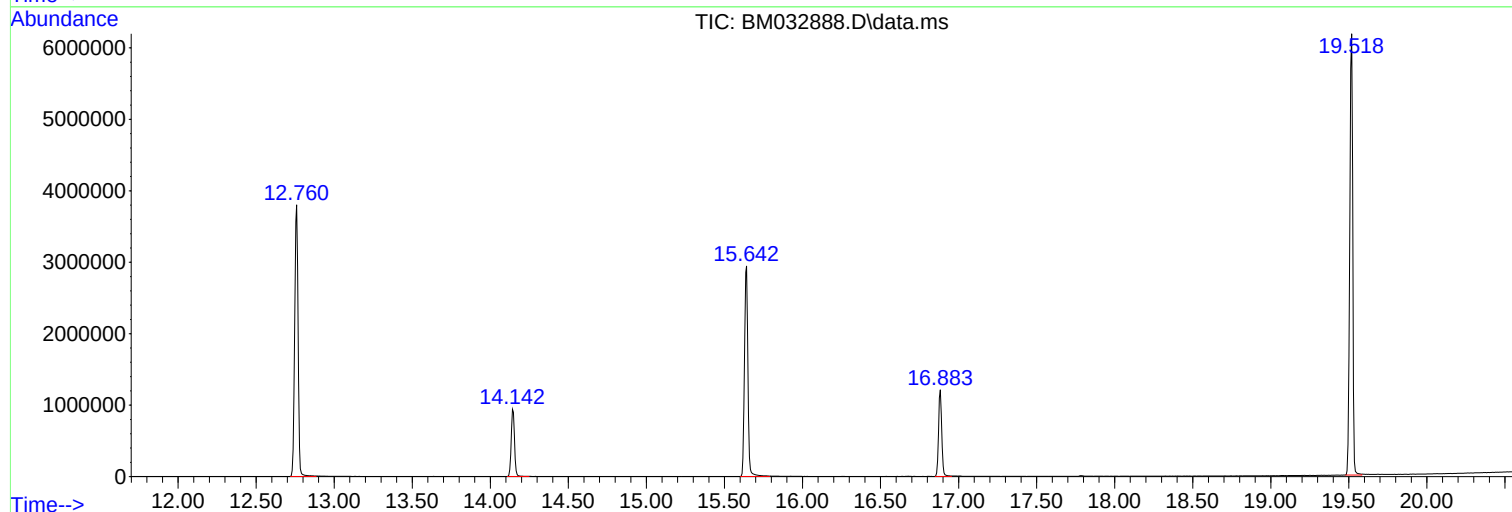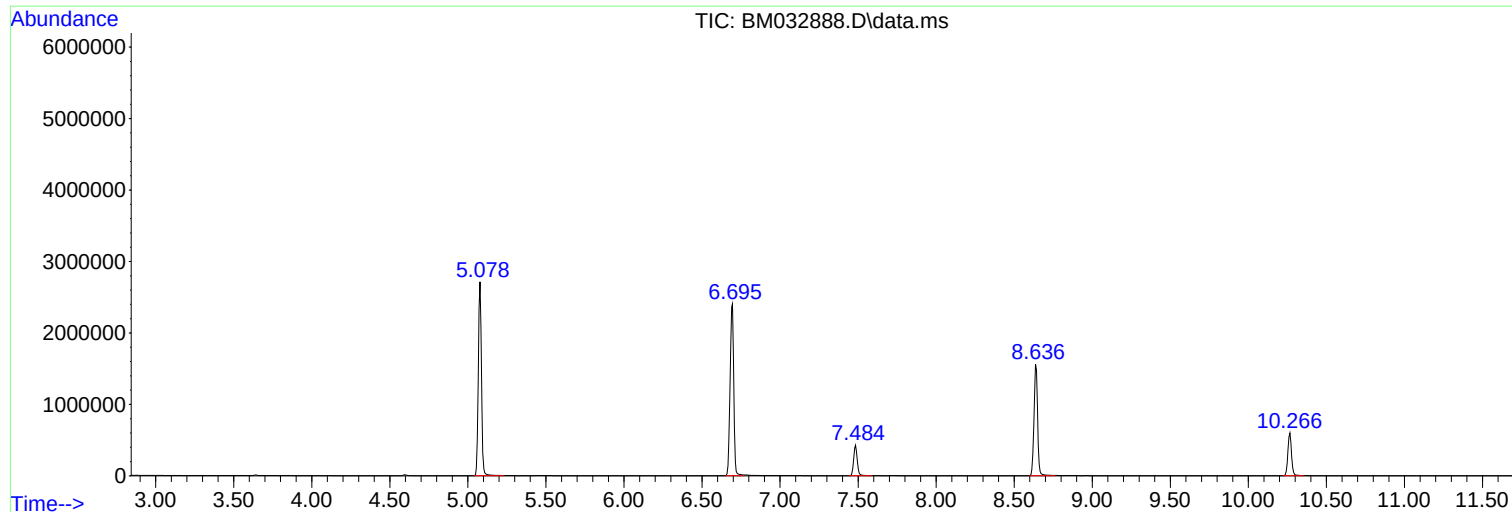

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110821\
Data File : BM032888.D
Acq On : 08 Nov 2021 10:59
Operator : CG/JU
Sample : PB140521BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140521BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110821\
Data File : BM032888.D
Acq On : 08 Nov 2021 10:59
Operator : CG/JU
Sample : PB140521BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB140521BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------