
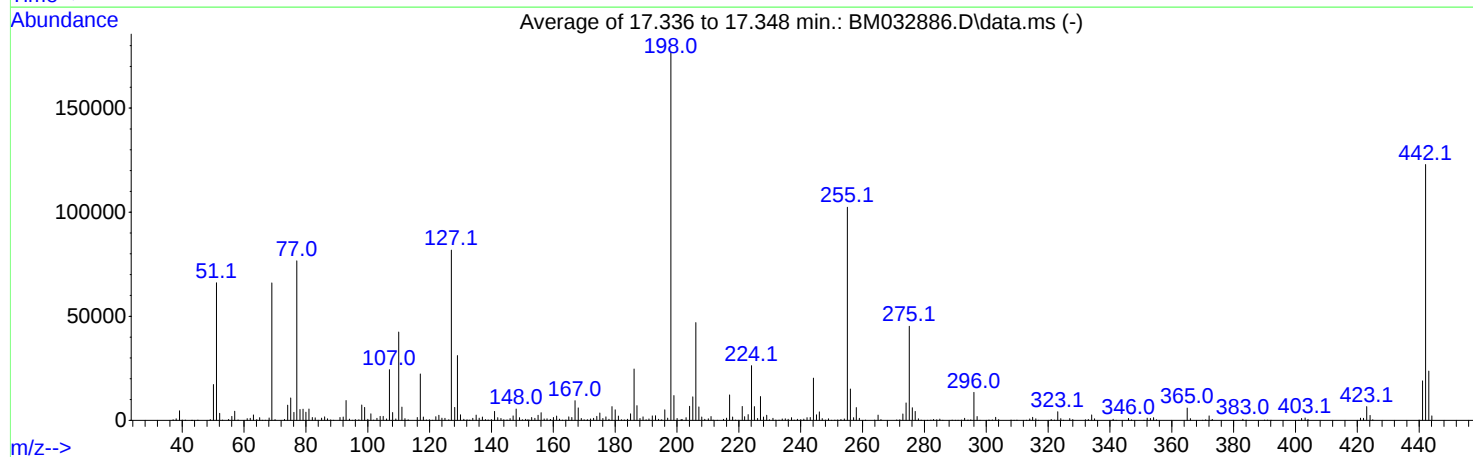


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110821\
 Data File : BM032886.D
 Acq On : 08 Nov 2021 09:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 02 16:07:18 2021

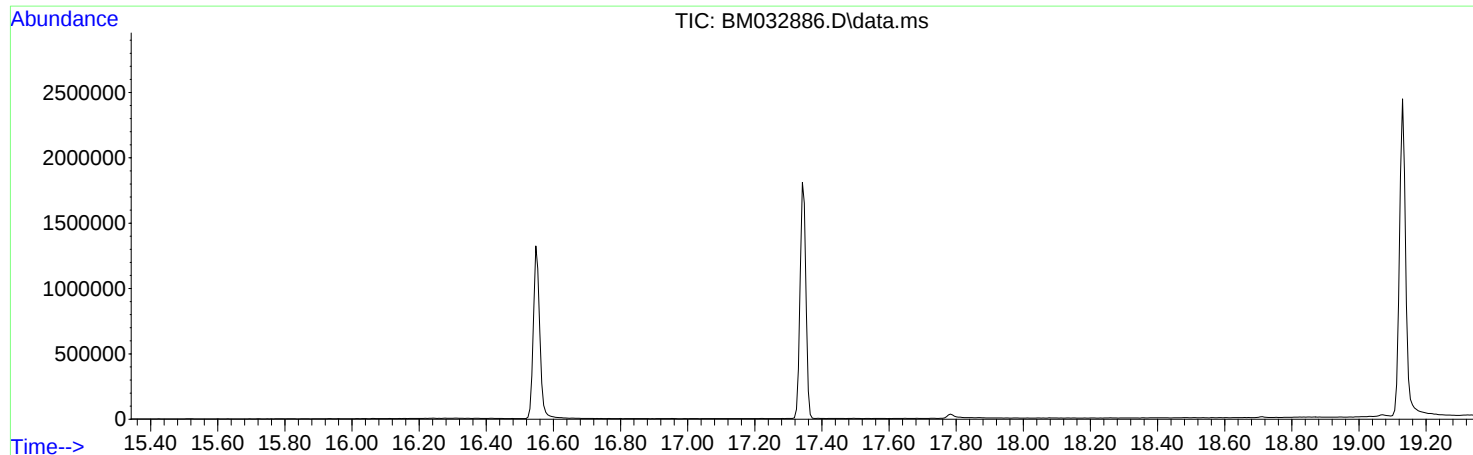




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	66099	PASS
68	69	0.00	2	1.8	1179	PASS
69	198	0.00	100	37.4	66059	PASS
70	69	0.00	2	0.6	372	PASS
127	198	10	80	46.3	81789	PASS
197	198	0.00	2	0.6	1071	PASS
198	198	100	100	100.0	176709	PASS
199	198	5	9	6.7	11914	PASS
275	198	10	60	25.6	45229	PASS
365	198	1	100	3.4	5958	PASS
441	198	0.01	100	10.8	19025	PASS
442	442	50	100	100.0	122917	PASS
443	442	15	24	19.3	23708	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110821\
Data File : BM032886.D
Acq On : 08 Nov 2021 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 08 11:17:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 16:07:18 2021
Response via : Initial Calibration

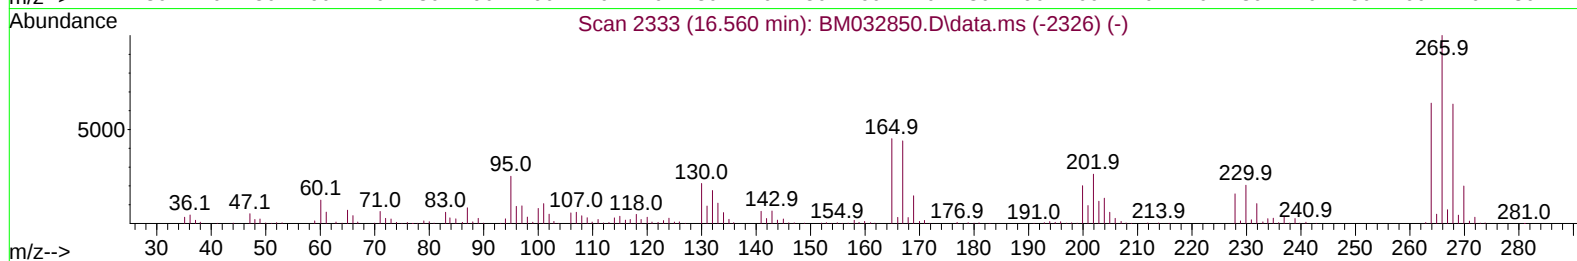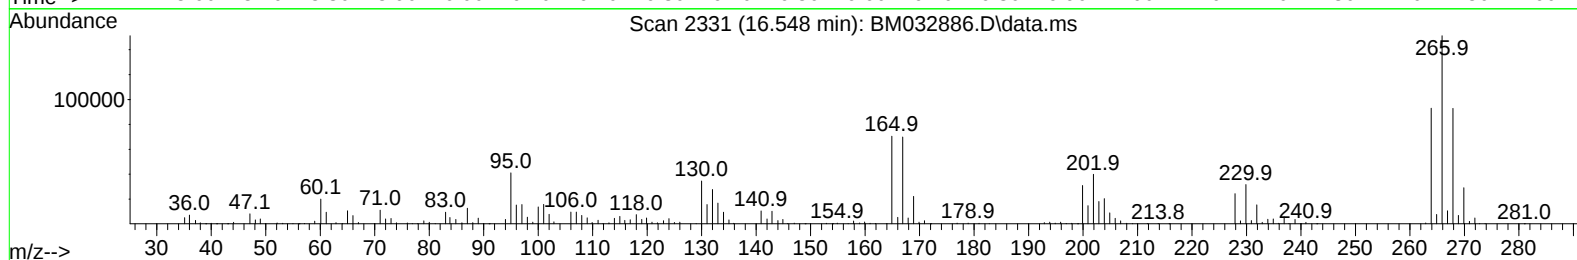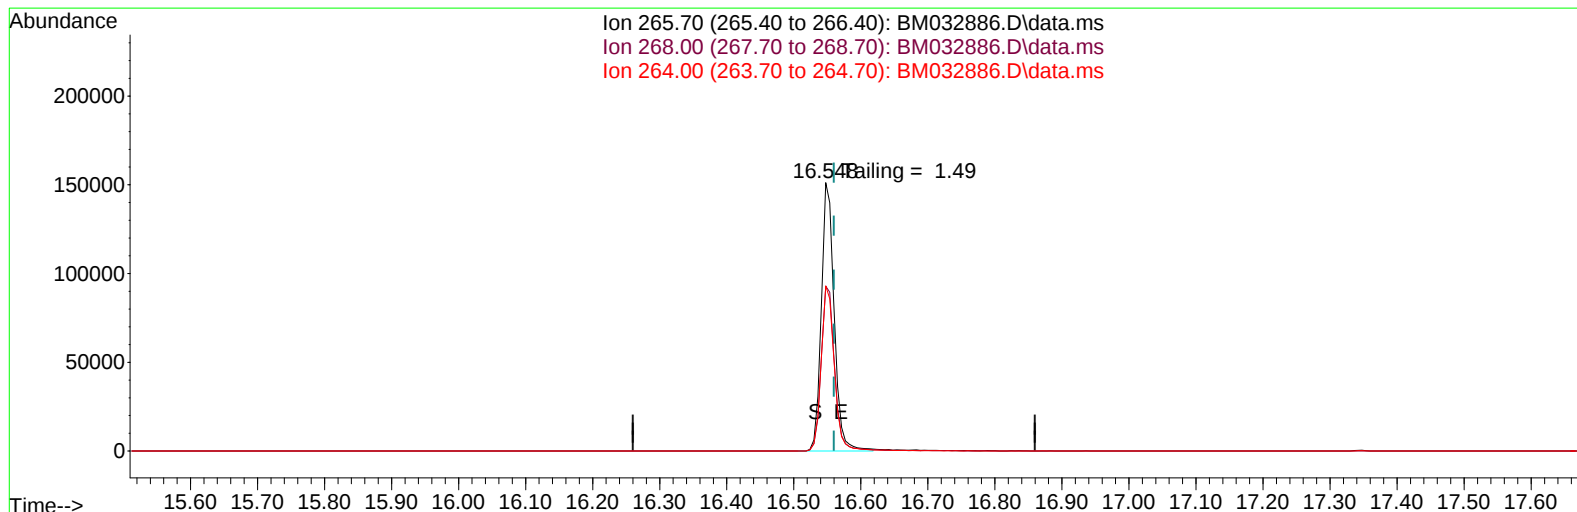

TIC: BM032886.D\data.ms

(70) Pentachlorophenol (C)

16.548min (-0.012) 0.00 ng




response 204349

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	61.41
264.00	65.10	61.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110821\
Data File : BM032886.D
Acq On : 08 Nov 2021 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 08 11:17:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM110221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 02 16:07:18 2021
Response via : Initial Calibration

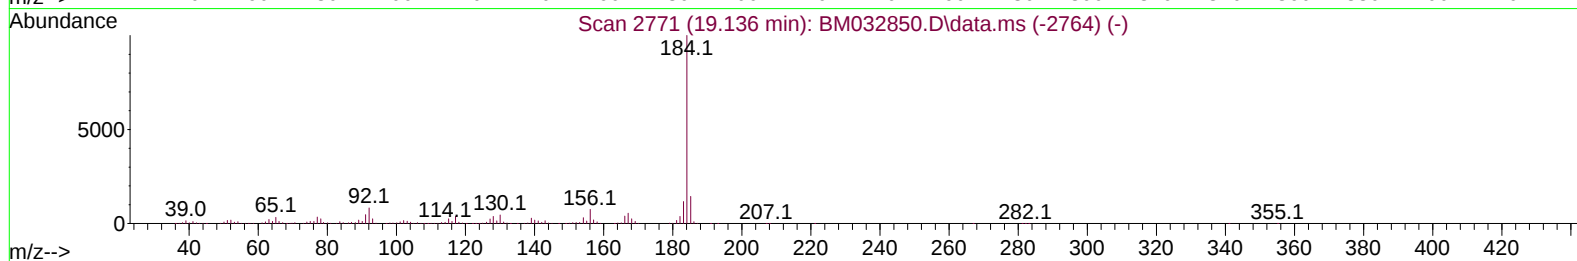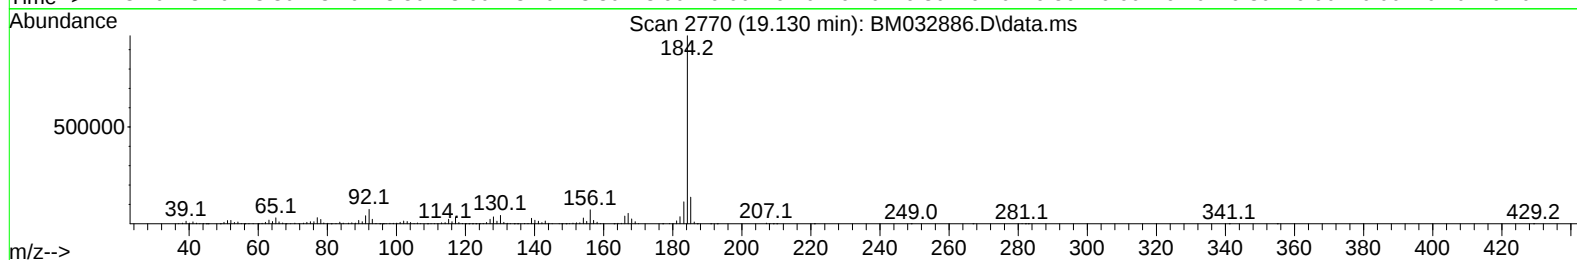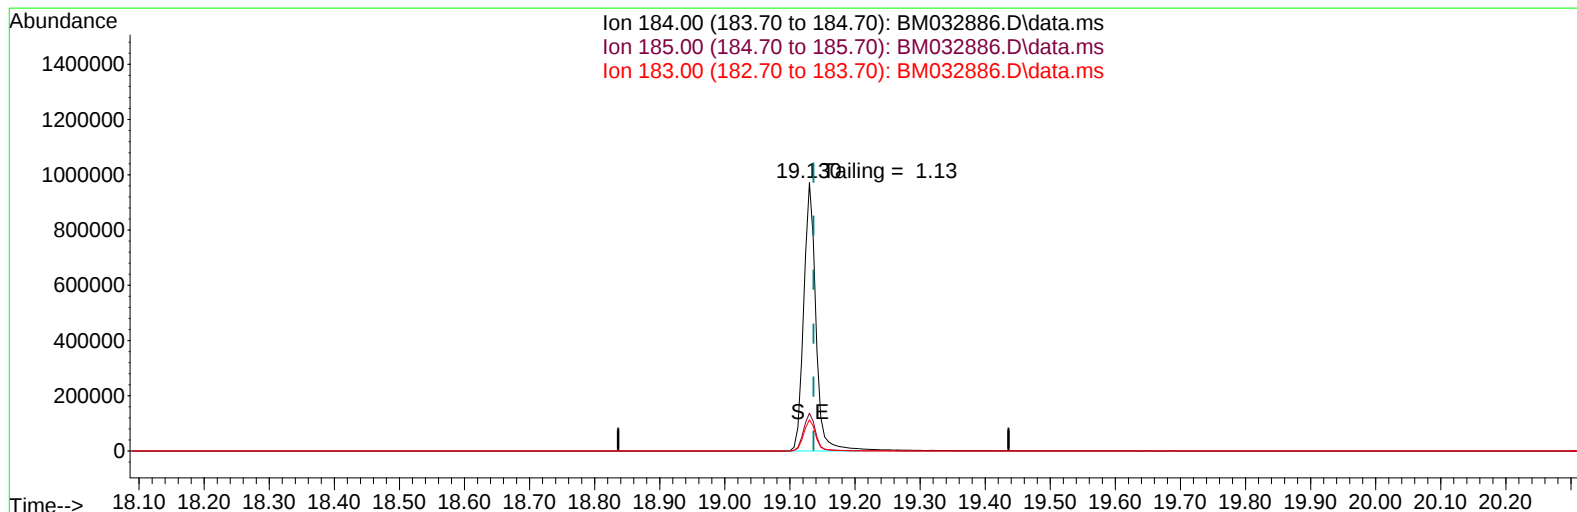

TIC: BM032886.D\data.ms

(77) Benzidine

19.130min (-0.006) 0.00 ng

response 1282605

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.15
183.00	11.20	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/8/2021	BNA_M	<u>BM032886.D</u>
Compound Name	Response	Retention Time
DDT	616251	20.37
DDD	9355	19.93
DDE	664	19.43
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10019	626270	1.60

Instrument :
BNA_M
ClientSampleId :
DFTPP