

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
 Data File : BM017571.D
 Acq On : 08 Nov 2018 18:01
 Operator : MJ/SJ
 Sample : J5834-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNR3

Quant Time: Nov 09 16:41:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 09 16:25:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	204588	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	904692	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	542060	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1341406	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1799335	20.00	ng/ul	0.00
86) Perylene-d12	23.42	264	1949651	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	31669	7.12	ng/uL	0.00
5) Phenol-d5	6.80	99	622856	33.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	404930	37.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	510443	35.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	525251	35.55	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	252987	35.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	277955	35.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	506634	34.40	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	728007	60.55	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1744388	37.53	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2090410	37.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	252745	29.10	ng/ul	0.00
58) Fluorene-d10	15.26	176	1537247	38.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	245346	26.25	ng/ul	0.00
71) Anthracene-d10	17.12	188	2503293	37.70	ng/ul	0.00
79) Pyrene-d10	19.42	212	3029377	36.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	3943590	38.30	ng/ul	0.00
Target Compounds						
6) Phenol	6.83	94	116590	6.283	ng/ul#	90
45) Dimethylphthalate	13.73	163	645236	14.327	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
Data File : BM017571.D
Acq On : 08 Nov 2018 18:01
Operator : MJ/SJ
Sample : J5834-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNR3

Quant Time: Nov 09 16:41:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 09 16:25:50 2018
Response via : Initial Calibration

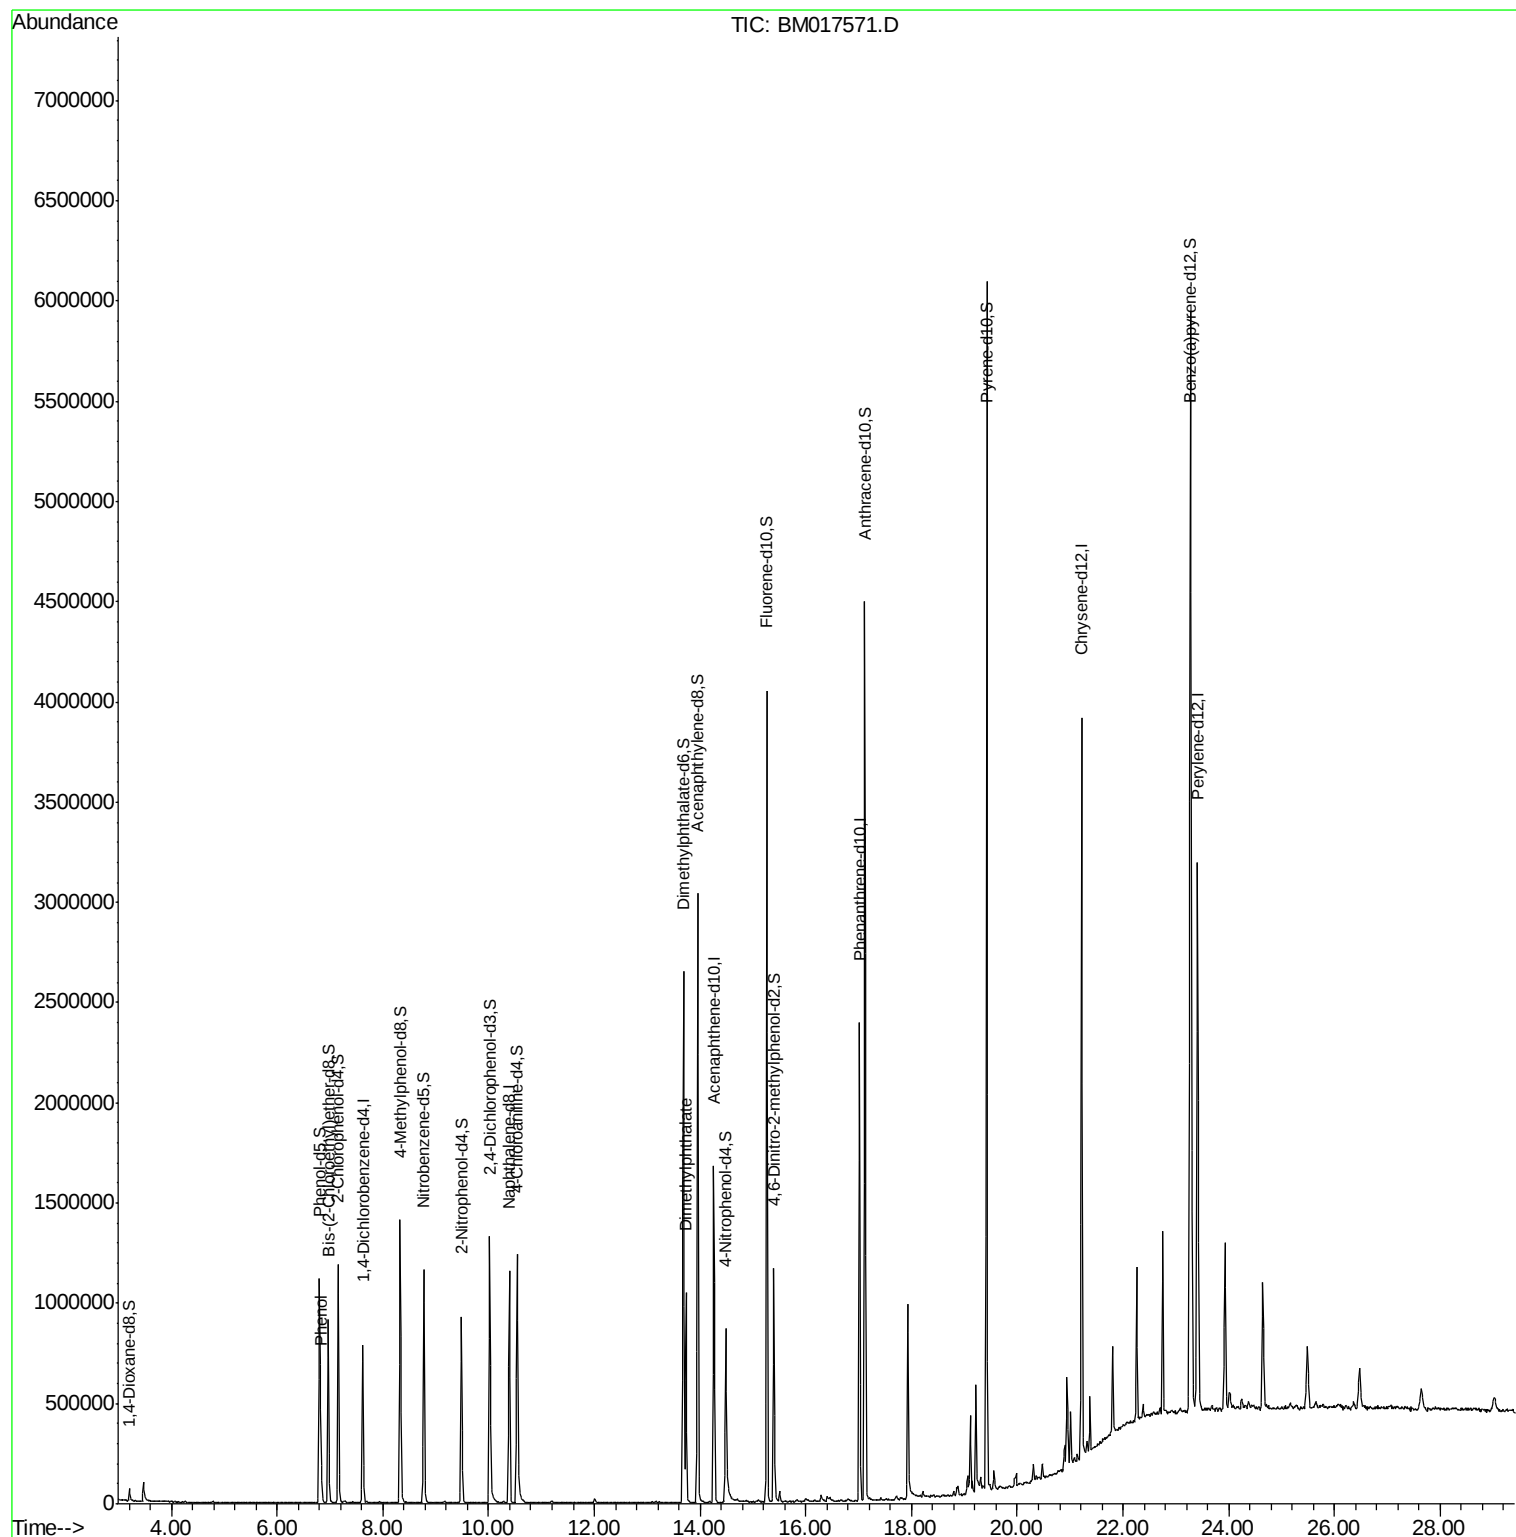

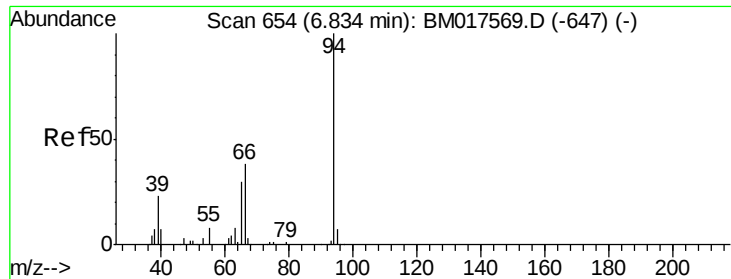

#6

Phenol

Concen: 6.283 ng/ul

RT: 6.83 min Scan# 653

Delta R.T. -0.01 min

Lab File: BM017571.D

Acq: 08 Nov 2018 18:01

Instrument :

BNA_M

ClientSampleId :

ESNR3





Tgt Ion: 94 Resp: 116590

Ion Ratio Lower Upper

94 100

65 31.8 24.0 36.0

66 48.0 31.1 46.7#

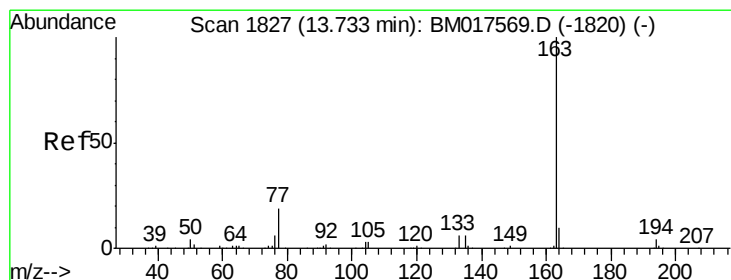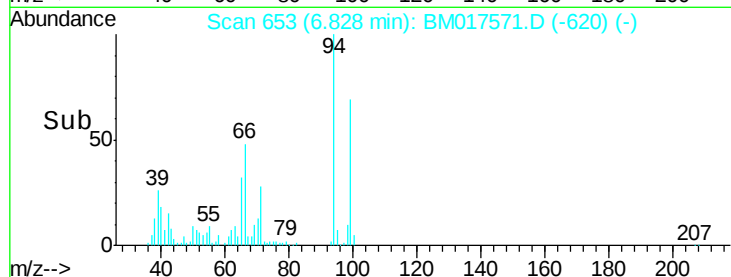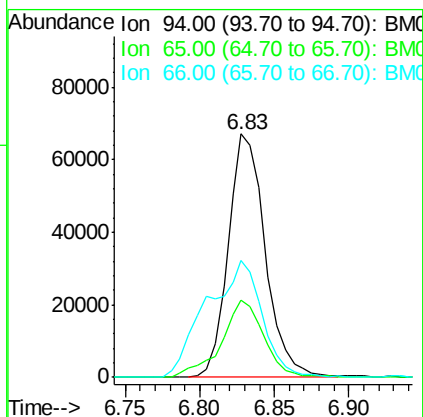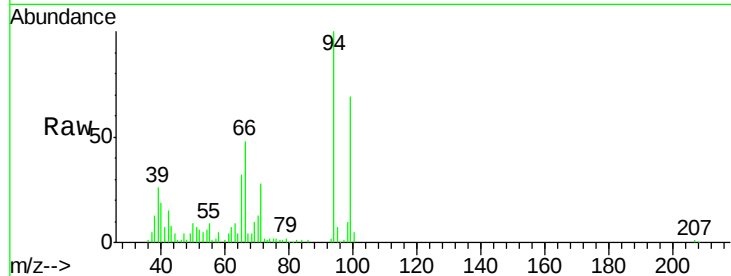

#45

Dimethylphthalate

Concen: 14.327 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. 0.00 min

Lab File: BM017571.D

Acq: 08 Nov 2018 18:01

Tgt Ion: 163 Resp: 645236

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 9.9 8.1 12.1

