

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
 Data File : BM017573.D
 Acq On : 08 Nov 2018 19:13
 Operator : MJ/SJ
 Sample : J5834-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNQ4

Quant Time: Nov 09 16:44:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 09 16:25:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	210676	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	950385	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	580240	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1433274	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1843153	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	1997272	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	19157	4.18	ng/uL	0.00
5) Phenol-d5	6.80	99	378908	19.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	249506	22.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	312164	20.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	313398	20.60	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	152910	20.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	170603	20.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	286589	18.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	418132	33.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1147099	23.05	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1264404	20.93	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	124838	13.43	ng/ul	0.00
58) Fluorene-d10	15.26	176	952530	22.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	137177	13.74	ng/ul	0.00
71) Anthracene-d10	17.12	188	1561824	22.01	ng/ul	0.00
79) Pyrene-d10	19.42	212	1833825	21.48	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	2283533	21.65	ng/ul	0.00


Target Compounds					Qvalue
6) Phenol	6.83	94	84240	4.408	ng/ul 96
45) Dimethylphthalate	13.73	163	627592	13.018	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
Data File : BM017573.D
Acq On : 08 Nov 2018 19:13
Operator : MJ/SJ
Sample : J5834-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNQ4

Quant Time: Nov 09 16:44:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 09 16:25:50 2018
Response via : Initial Calibration

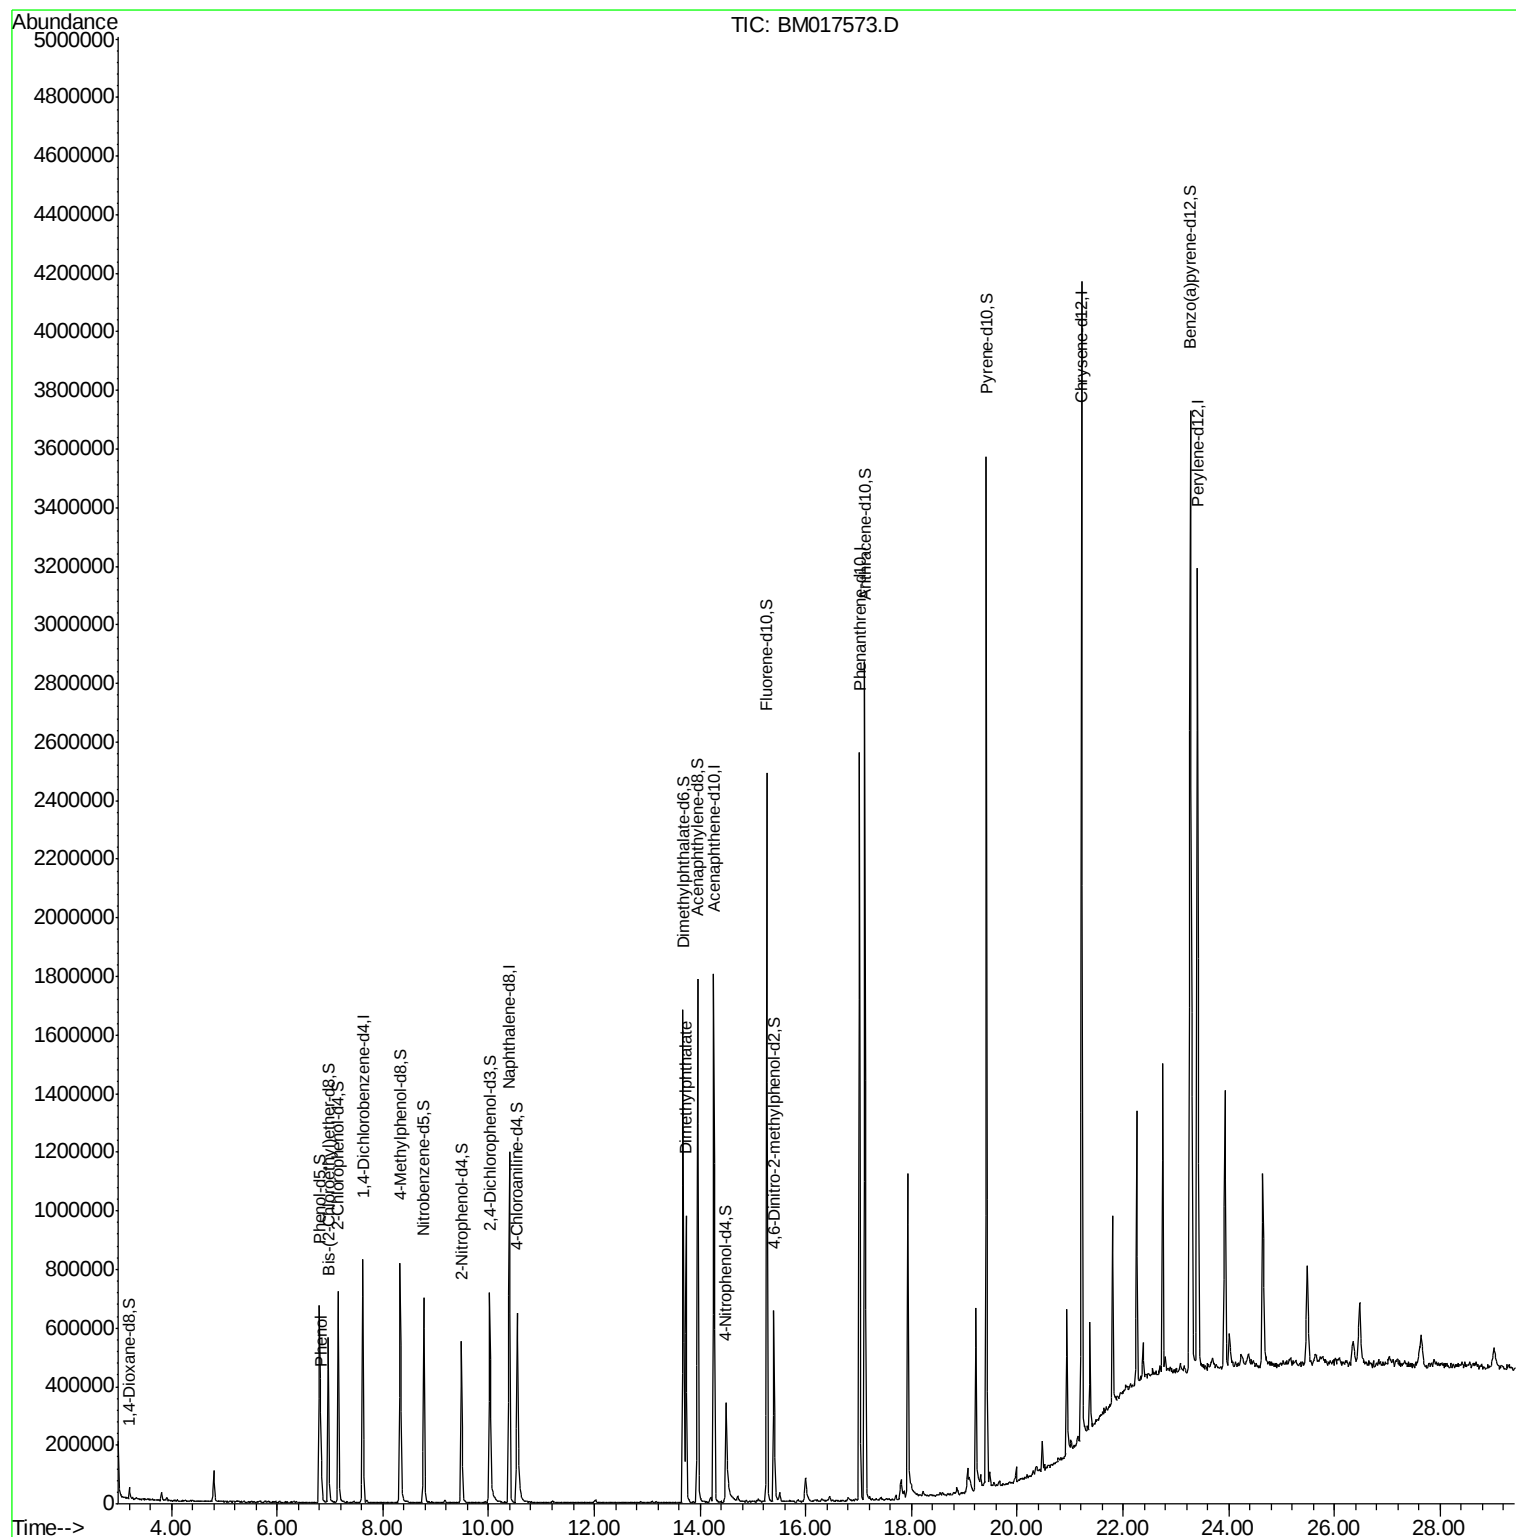

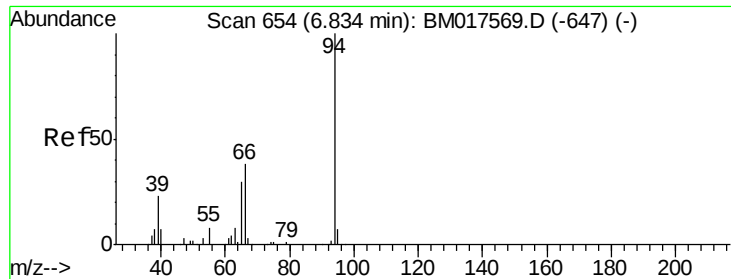

#6

Phenol

Concen: 4.408 ng/ul

RT: 6.83 min Scan# 654

Delta R.T. 0.00 min

Lab File: BM017573.D

Acq: 08 Nov 2018 19:13

Instrument :

BNA_M

ClientSampleId :

ESNQ4





Tgt Ion: 94 Resp: 84240

Ion Ratio Lower Upper

94 100

65 31.3 24.0 36.0

66 42.0 31.1 46.7

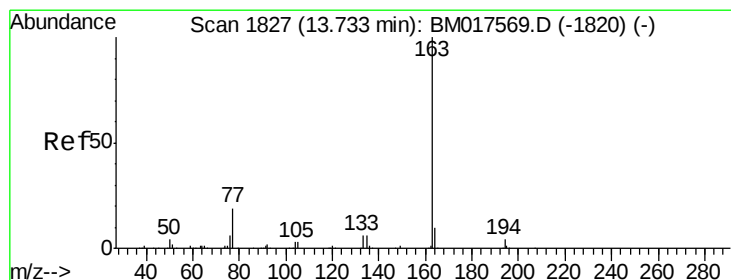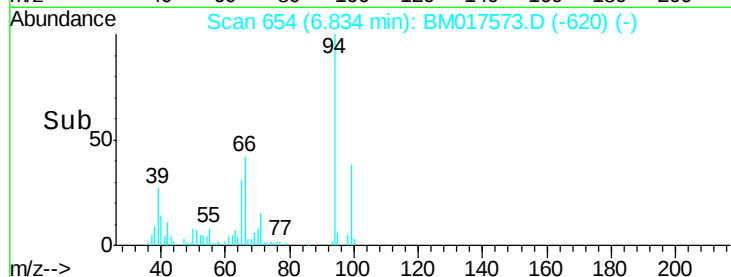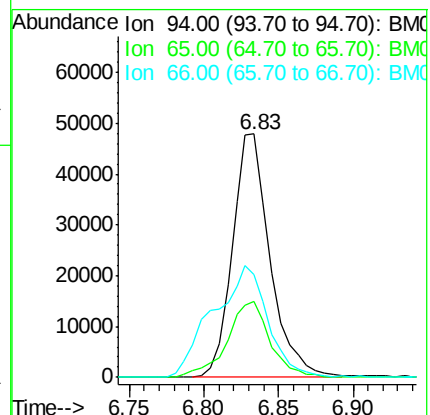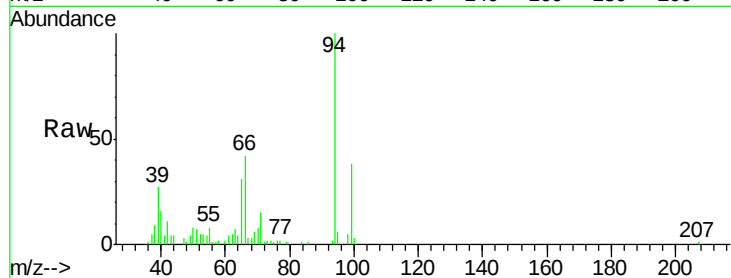

#45

Dimethylphthalate

Concen: 13.018 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. 0.00 min

Lab File: BM017573.D

Acq: 08 Nov 2018 19:13

Tgt Ion: 163 Resp: 627592

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 9.8 8.1 12.1

