

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
 Data File : BM017581.D
 Acq On : 09 Nov 2018 00:00
 Operator : MJ/SJ
 Sample : J5834-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNR6

Quant Time: Nov 09 17:01:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 09 16:25:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	219745	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	984739	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	604602	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1463857	20.00	ng/ul	0.00
78) Chrysene-d12	21.21	240	1882797	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	2023663	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	25832	5.41	ng/uL	0.00
5) Phenol-d5	6.80	99	534768	26.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	355110	30.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	433365	27.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	444055	27.98	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	222545	28.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	247313	28.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	410886	25.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	620768	47.43	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1585935	30.59	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1791905	28.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	218883	22.60	ng/ul	0.00
58) Fluorene-d10	15.26	176	1333330	29.61	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	234443	22.99	ng/ul	0.00
71) Anthracene-d10	17.12	188	2116522	29.21	ng/ul	0.00
79) Pyrene-d10	19.42	212	2506458	28.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	3062274	28.65	ng/ul	0.00
Target Compounds						
6) Phenol	6.83	94	110683	5.553	ng/ul	92
45) Dimethylphthalate	13.73	163	577058	11.488	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
Data File : BM017581.D
Acq On : 09 Nov 2018 00:00
Operator : MJ/SJ
Sample : J5834-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
ESNR6

Quant Time: Nov 09 17:01:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 09 16:25:50 2018
Response via : Initial Calibration

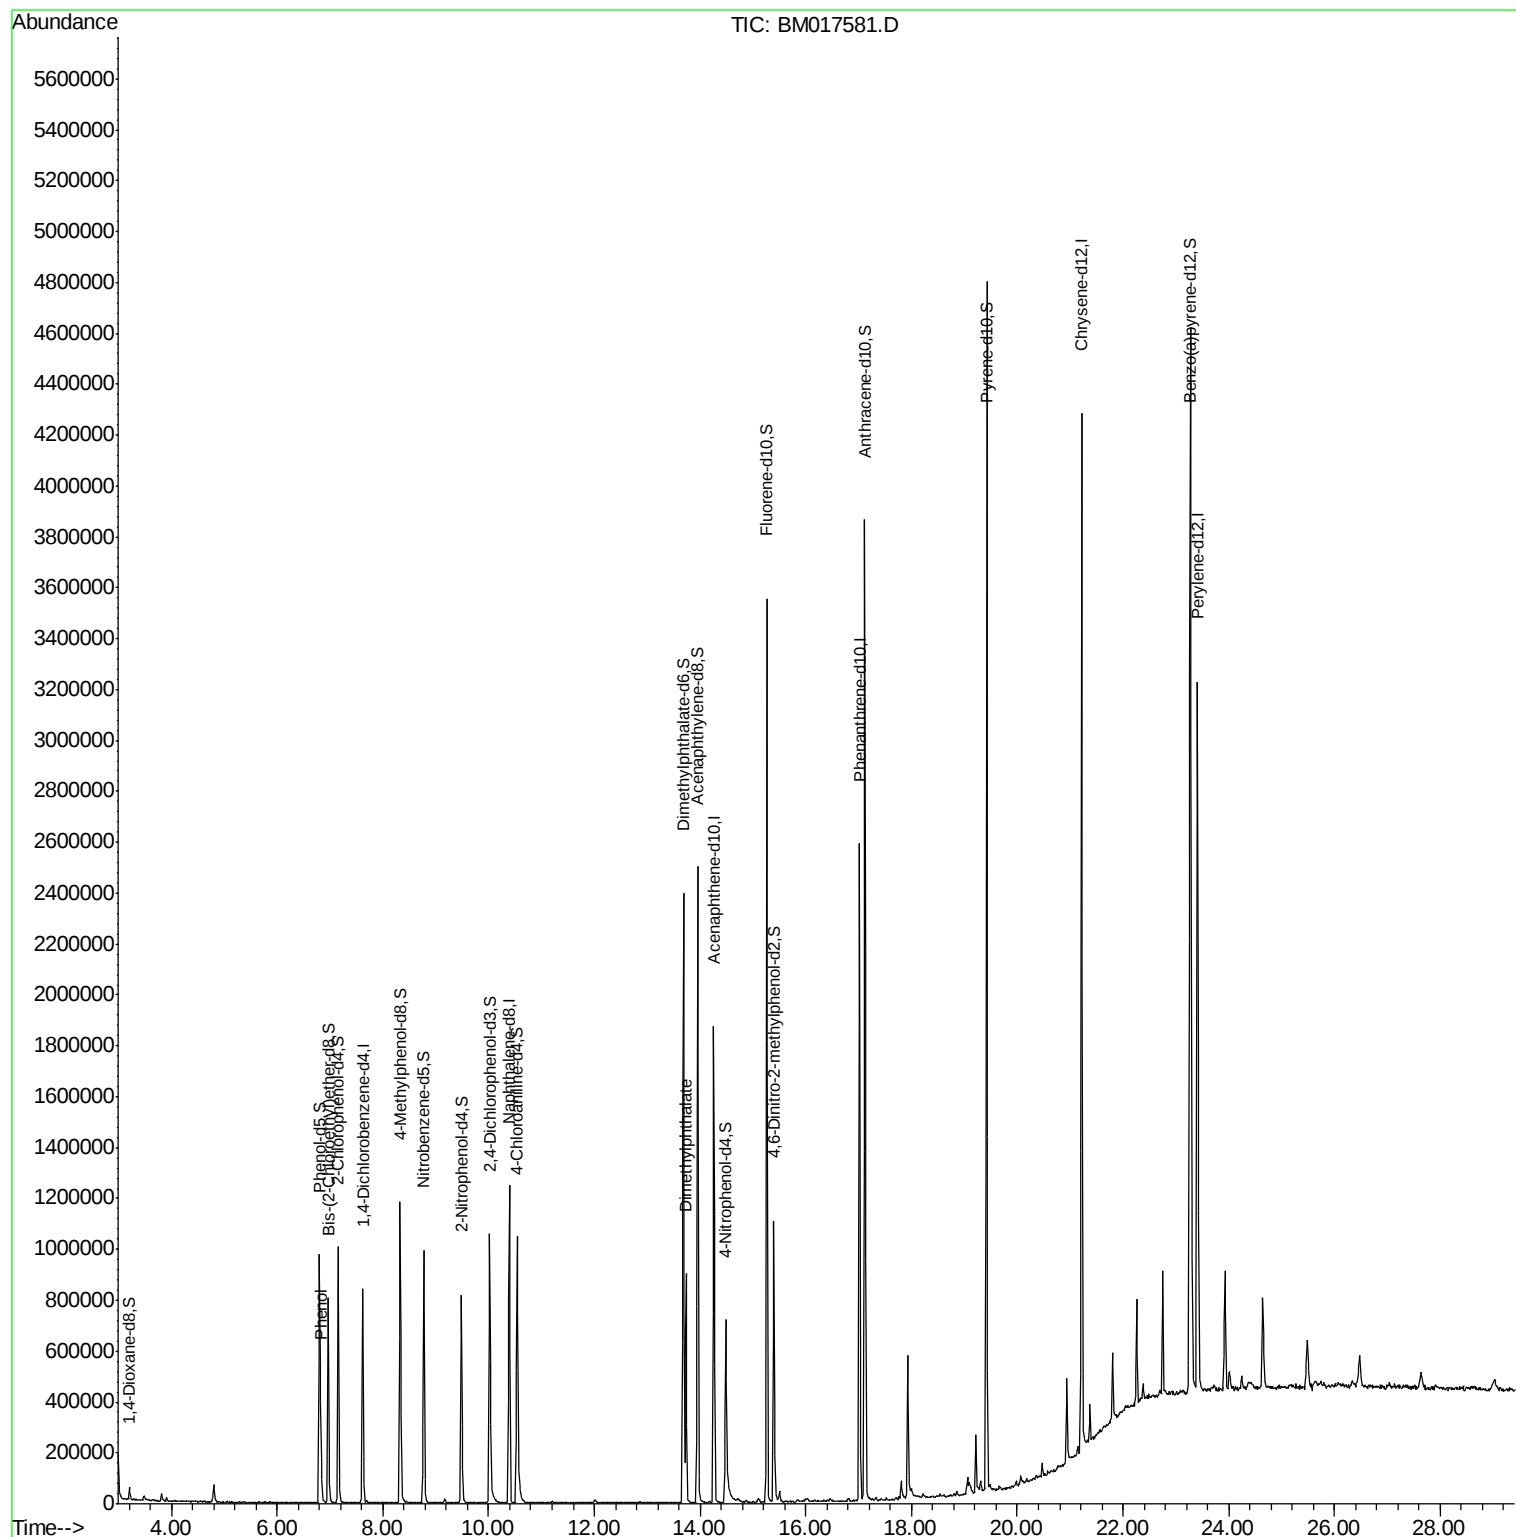

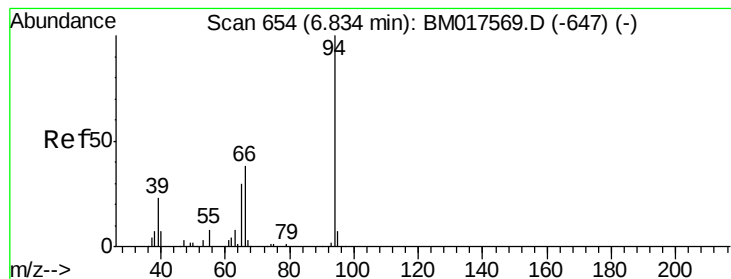

#6

Phenol

Concen: 5.553 ng/ul

RT: 6.83 min Scan# 653

Delta R.T. -0.01 min

Lab File: BM017581.D

Acq: 09 Nov 2018 00:00

Instrument :

BNA_M

ClientSampleId :

ESNR6





Tgt Ion: 94 Resp: 110683

Ion Ratio Lower Upper

94 100

65 31.0 24.0 36.0

66 46.4 31.1 46.7

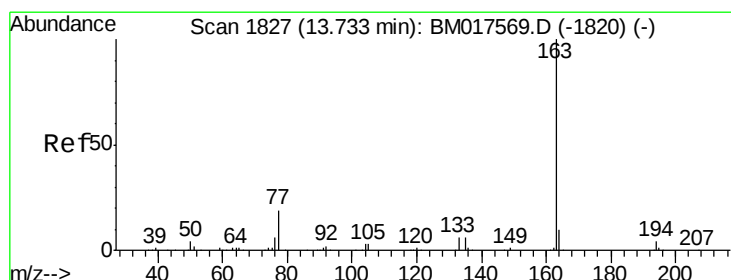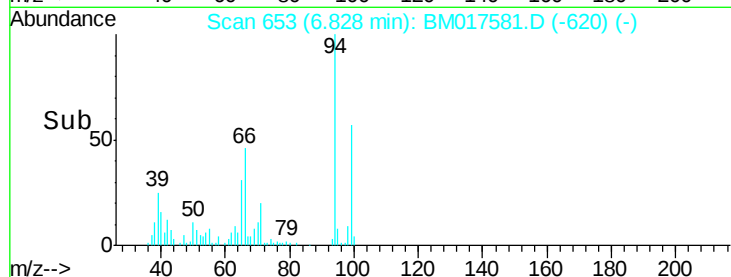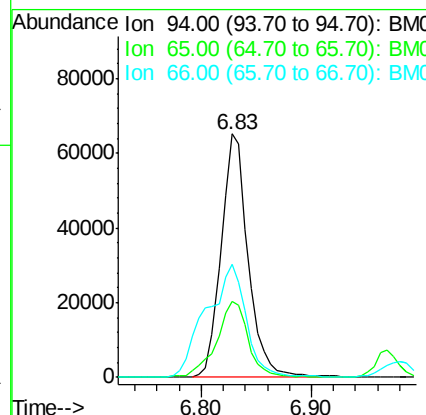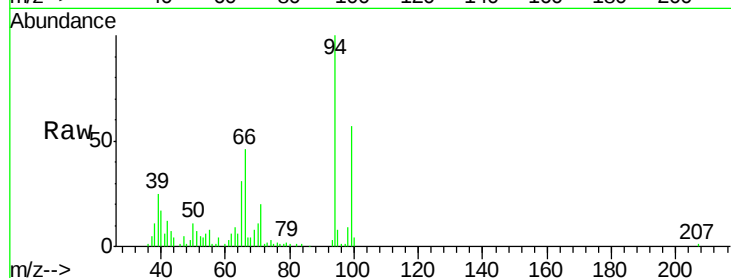

#45

Dimethylphthalate

Concen: 11.488 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. -0.00 min

Lab File: BM017581.D

Acq: 09 Nov 2018 00:00

Tgt Ion: 163 Resp: 577058

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.3 8.1 12.1

