

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
 Data File : BM017582.D
 Acq On : 09 Nov 2018 00:36
 Operator : MJ/SJ
 Sample : J5834-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNR1

Quant Time: Nov 09 17:03:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 09 16:25:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	239612	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1054232	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	651652	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1581424	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1937154	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	2046260	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	21191	4.07	ng/uL	0.00
5) Phenol-d5	6.80	99	397561	18.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	284075	22.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	338671	19.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	306942	17.74	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	177683	21.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	199844	21.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	333480	19.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	510887	36.46	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1338521	23.95	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1534221	22.61	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	185392	17.76	ng/ul	0.00
58) Fluorene-d10	15.26	176	1153996	23.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	191343	17.37	ng/ul	0.00
71) Anthracene-d10	17.12	188	1846966	23.59	ng/ul	0.00
79) Pyrene-d10	19.42	212	2197909	24.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	2626704	24.31	ng/ul	0.00
Target Compounds						
6) Phenol	6.83	94	78558	3.615	ng/ul	94
45) Dimethylphthalate	13.73	163	399469	7.378	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
Data File : BM017582.D
Acq On : 09 Nov 2018 00:36
Operator : MJ/SJ
Sample : J5834-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNR1

Quant Time: Nov 09 17:03:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 09 16:25:50 2018
Response via : Initial Calibration

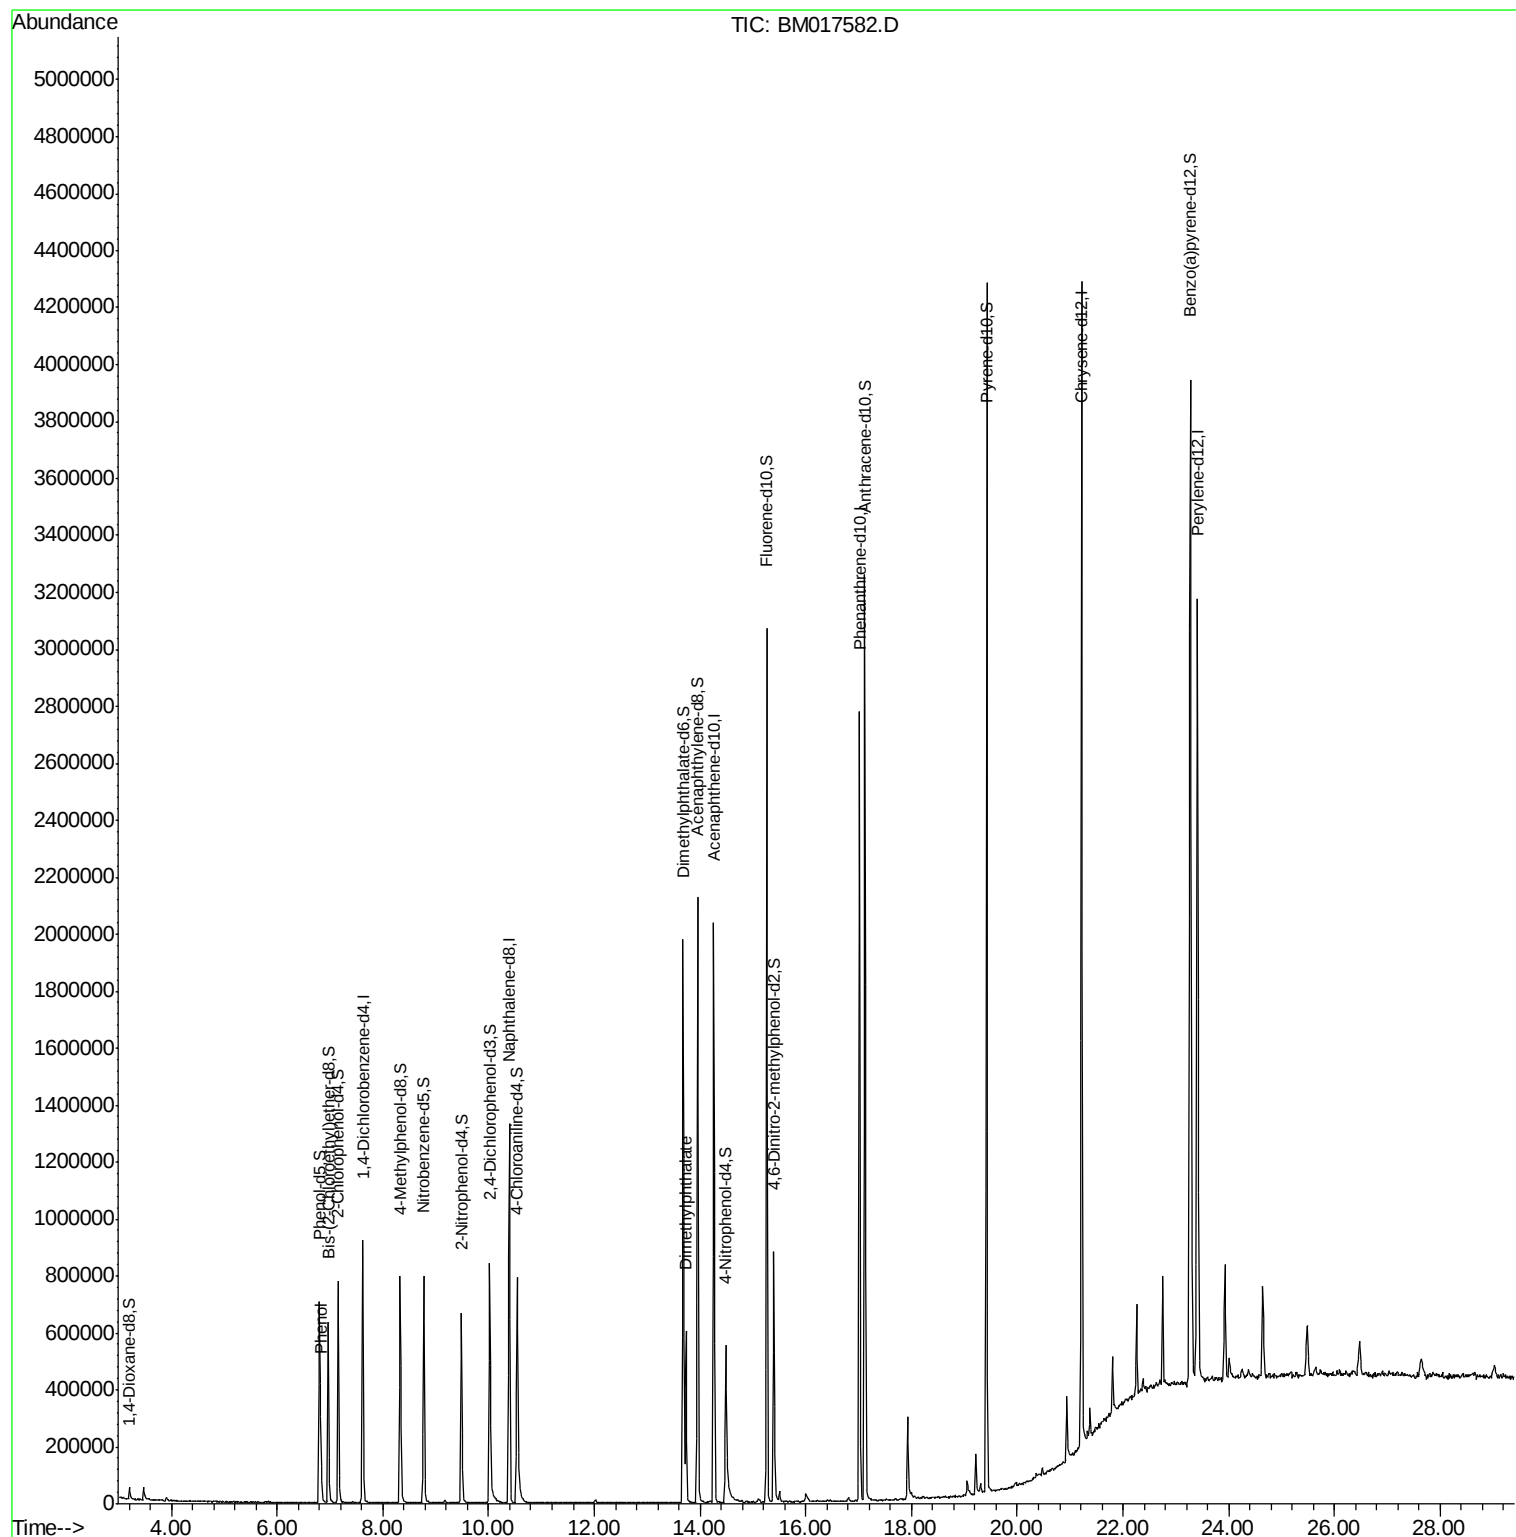

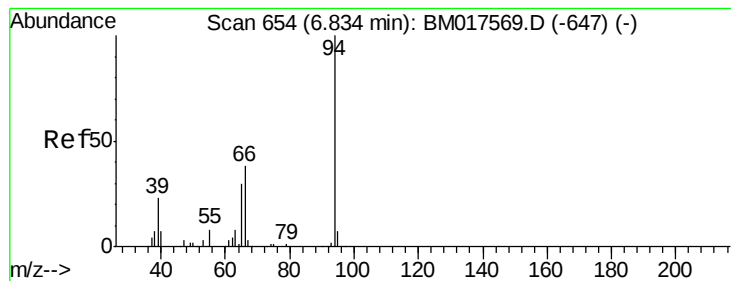

#6

Phenol

Concen: 3.615 ng/ul

RT: 6.83 min Scan# 653

Delta R.T. -0.01 min

Lab File: BM017582.D

Acq: 09 Nov 2018 00:36

Instrument :

BNA_M

ClientSampleId :

ESNR1





Tgt Ion: 94 Resp: 78558

Ion Ratio Lower Upper

94 100

65 30.8 24.0 36.0

66 44.8 31.1 46.7

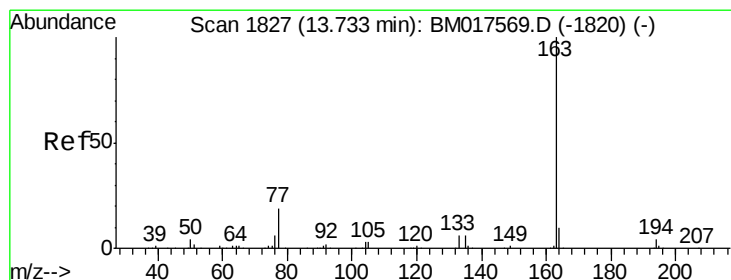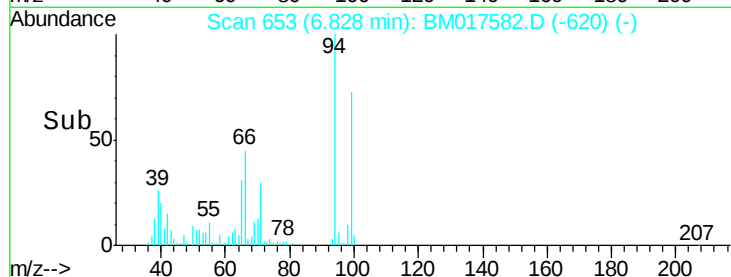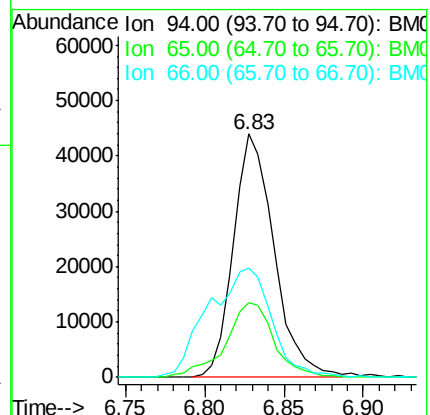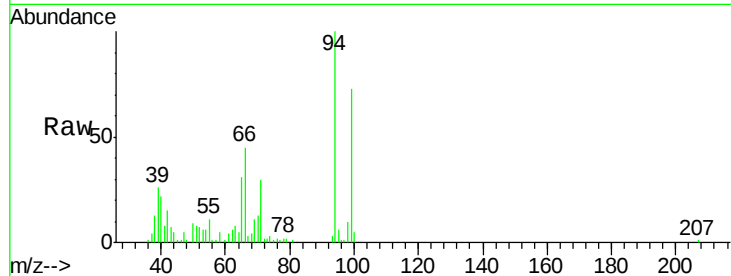

#45

Dimethylphthalate

Concen: 7.378 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. -0.00 min

Lab File: BM017582.D

Acq: 09 Nov 2018 00:36

Tgt Ion: 163 Resp: 399469

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.2 8.1 12.1

