

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
 Data File : BM017583.D
 Acq On : 09 Nov 2018 01:11
 Operator : MJ/SJ
 Sample : J5834-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNR7

Quant Time: Nov 09 17:04:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 09 16:25:50 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	237310	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1067350	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	650749	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1560133	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	1945471	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	2098053	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	30058	5.83	ng/uL	0.00
5) Phenol-d5	6.80	99	654877	30.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	422158	33.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	525630	31.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	553414	32.29	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	274775	32.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	313597	33.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	545213	31.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	805216	56.76	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	2099359	37.62	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2456992	36.26	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	329679	31.62	ng/ul	0.00
58) Fluorene-d10	15.26	176	1802490	37.19	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	328860	30.25	ng/ul	0.00
71) Anthracene-d10	17.12	188	2918736	37.79	ng/ul	0.00
79) Pyrene-d10	19.42	212	3471592	38.52	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	4327502	39.06	ng/ul	0.00
Target Compounds						
6) Phenol	6.83	94	118881	5.523	ng/ul	94
45) Dimethylphthalate	13.73	163	690782	12.776	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
Data File : BM017583.D
Acq On : 09 Nov 2018 01:11
Operator : MJ/SJ
Sample : J5834-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNR7

Quant Time: Nov 09 17:04:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 09 16:25:50 2018
Response via : Initial Calibration

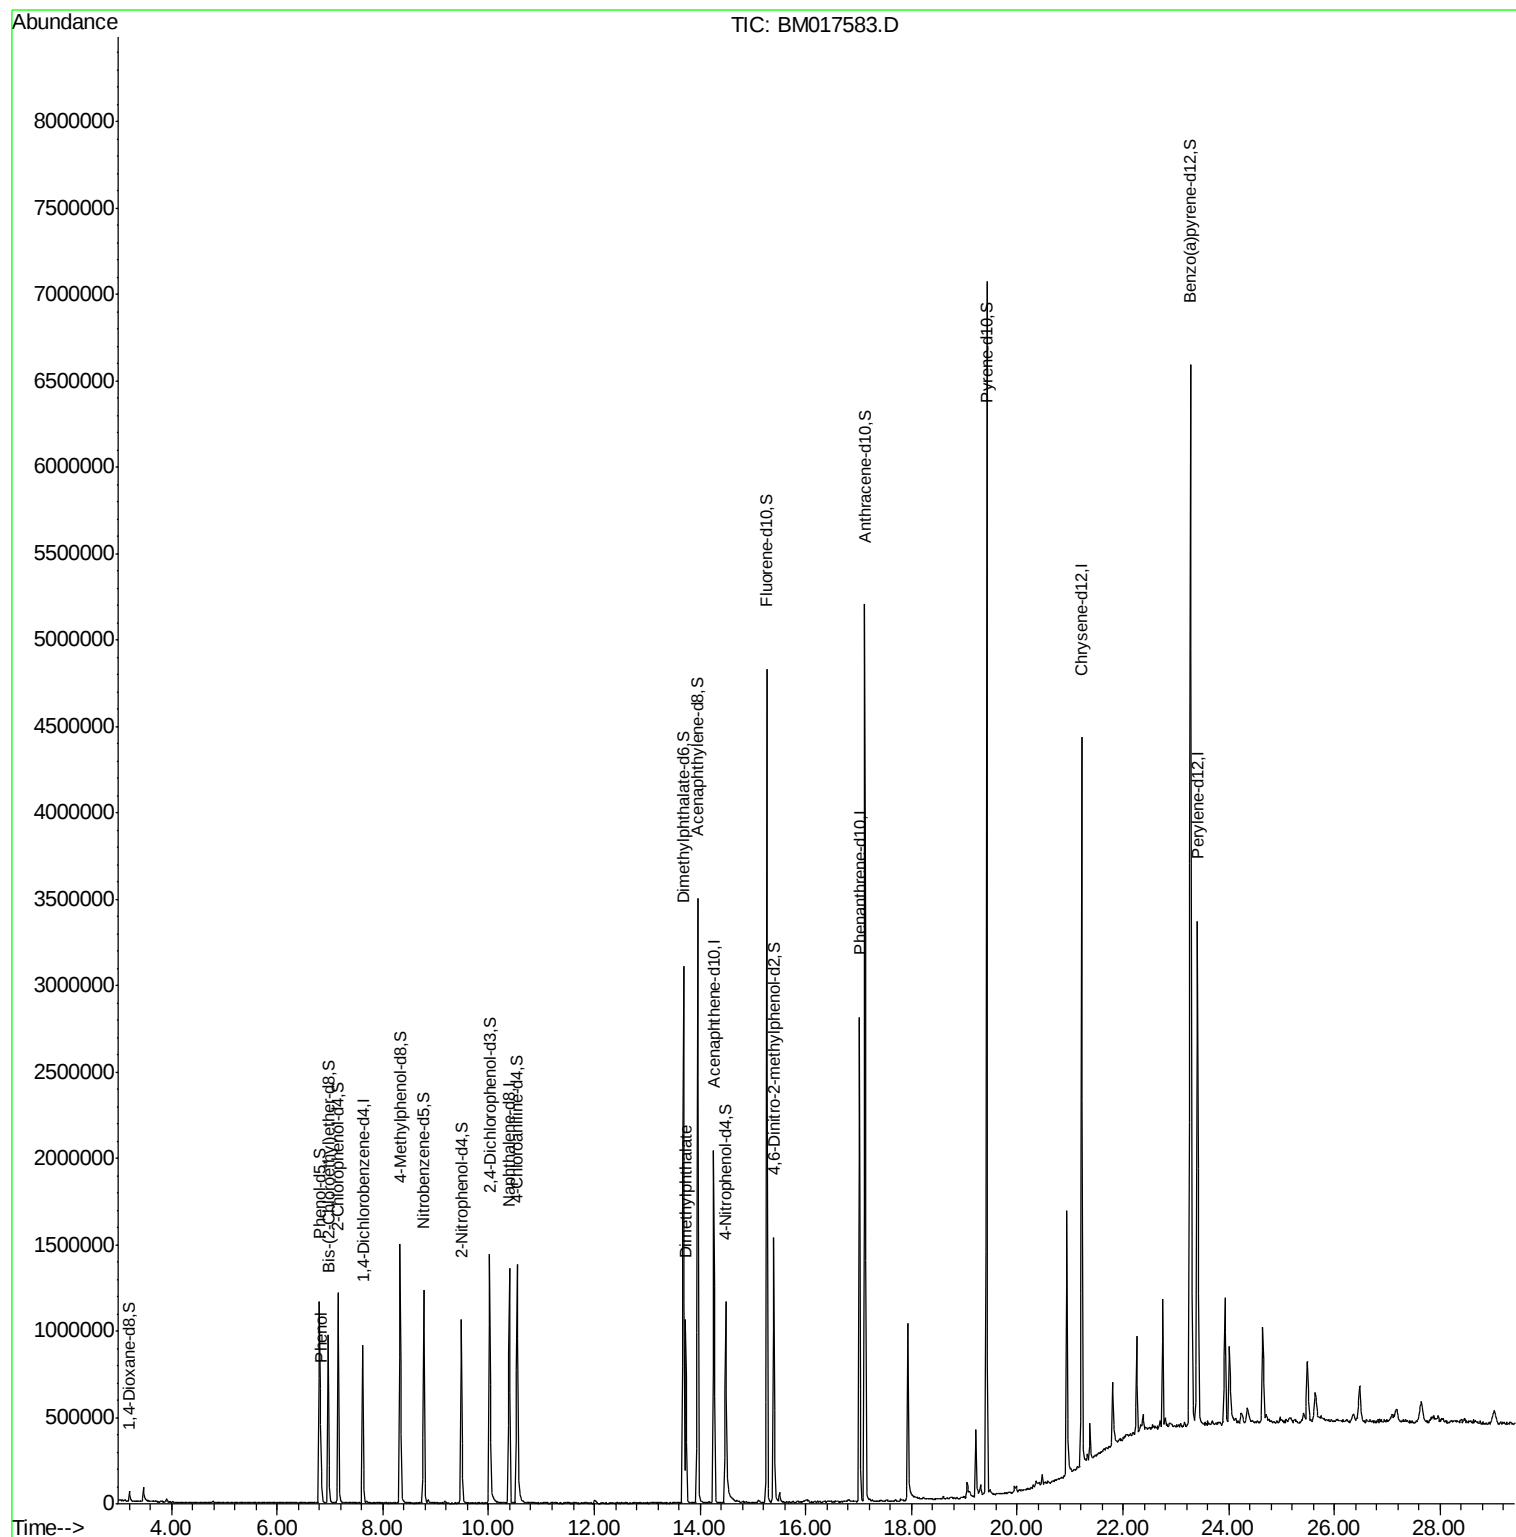

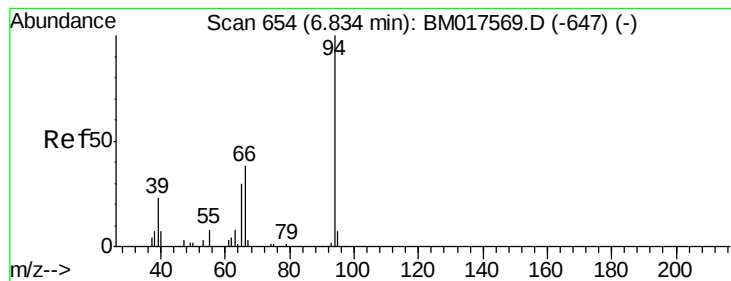

#6

Phenol

Concen: 5.523 ng/ul

RT: 6.83 min Scan# 653

Delta R.T. -0.01 min

Lab File: BM017583.D

Acq: 09 Nov 2018 01:11

Instrument :

BNA_M

ClientSampleId :

ESNR7


Tgt Ion: 94 Resp: 118881

Ion Ratio Lower Upper

94 100

65 31.8 24.0 36.0




66 44.2 31.1 46.7

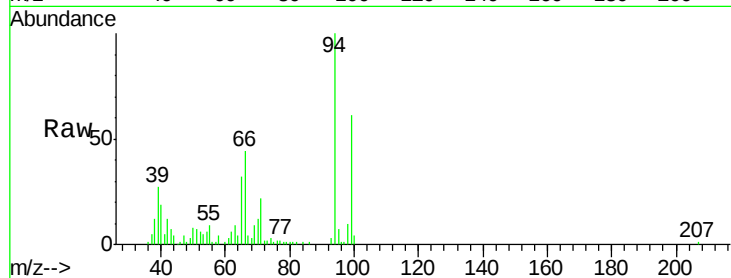

Abundance Ion 94.00 (93.70 to 94.70): BM017569.D (-647) (-)

Ion 65.00 (64.70 to 65.70): BM017569.D (-647) (-)

Ion 66.00 (65.70 to 66.70): BM017569.D (-647) (-)

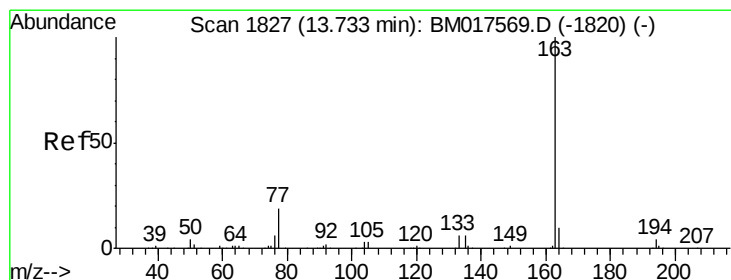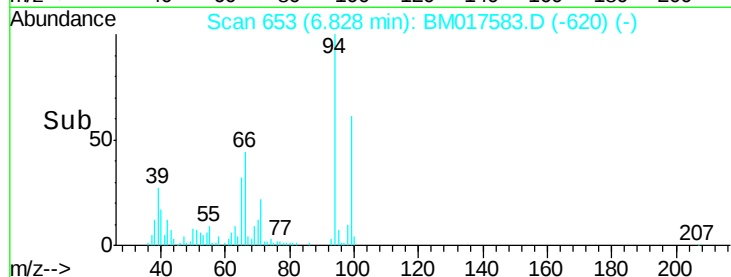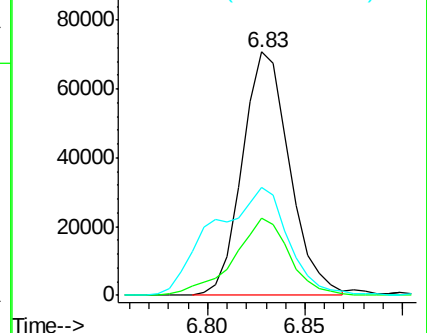

#45

Dimethylphthalate

Concen: 12.776 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. -0.00 min

Lab File: BM017583.D

Acq: 09 Nov 2018 01:11


Tgt Ion: 163 Resp: 690782

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.2 8.1 12.1

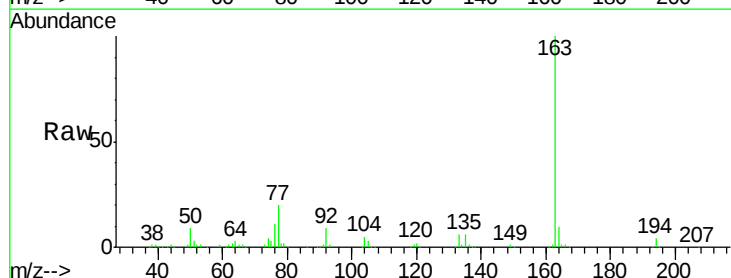

Abundance Ion 163.00 (162.70 to 163.70): BM017569.D (-1820) (-)

Ion 194.00 (193.70 to 194.70): BM017569.D (-1820) (-)

Ion 164.00 (163.70 to 164.70): BM017569.D (-1820) (-)

