

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
 Data File : BM017586.D
 Acq On : 09 Nov 2018 03:35
 Operator : MJ/SJ
 Sample : J5834-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ESNS4

Quant Time: Nov 09 17:09:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 09 16:25:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	269944	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	1198123	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.26	164	743517	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	1819437	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	2252597	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	2297023	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	30628	5.22	ng/uL	0.00
5) Phenol-d5	6.80	99	687521	27.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	450704	31.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	566601	29.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	587234	30.12	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	288061	30.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	326438	31.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	574002	29.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	856002	53.76	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	2215400	34.75	ng/ul	0.00
47) Acenaphthylene-d8	13.95	160	2514307	32.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	346616	29.10	ng/ul	0.00
58) Fluorene-d10	15.26	176	1866213	33.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	323102	25.49	ng/ul	0.00
71) Anthracene-d10	17.12	188	3074382	34.14	ng/ul	0.00
79) Pyrene-d10	19.42	212	3643699	34.91	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	4254647	35.07	ng/ul	0.00


Target Compounds						Qvalue
6) Phenol	6.83	94	96504	3.941	ng/ul	94
45) Dimethylphthalate	13.73	163	521414	8.440	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM110918\
Data File : BM017586.D
Acq On : 09 Nov 2018 03:35
Operator : MJ/SJ
Sample : J5834-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ESNS4

Quant Time: Nov 09 17:09:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 09 16:25:50 2018
Response via : Initial Calibration

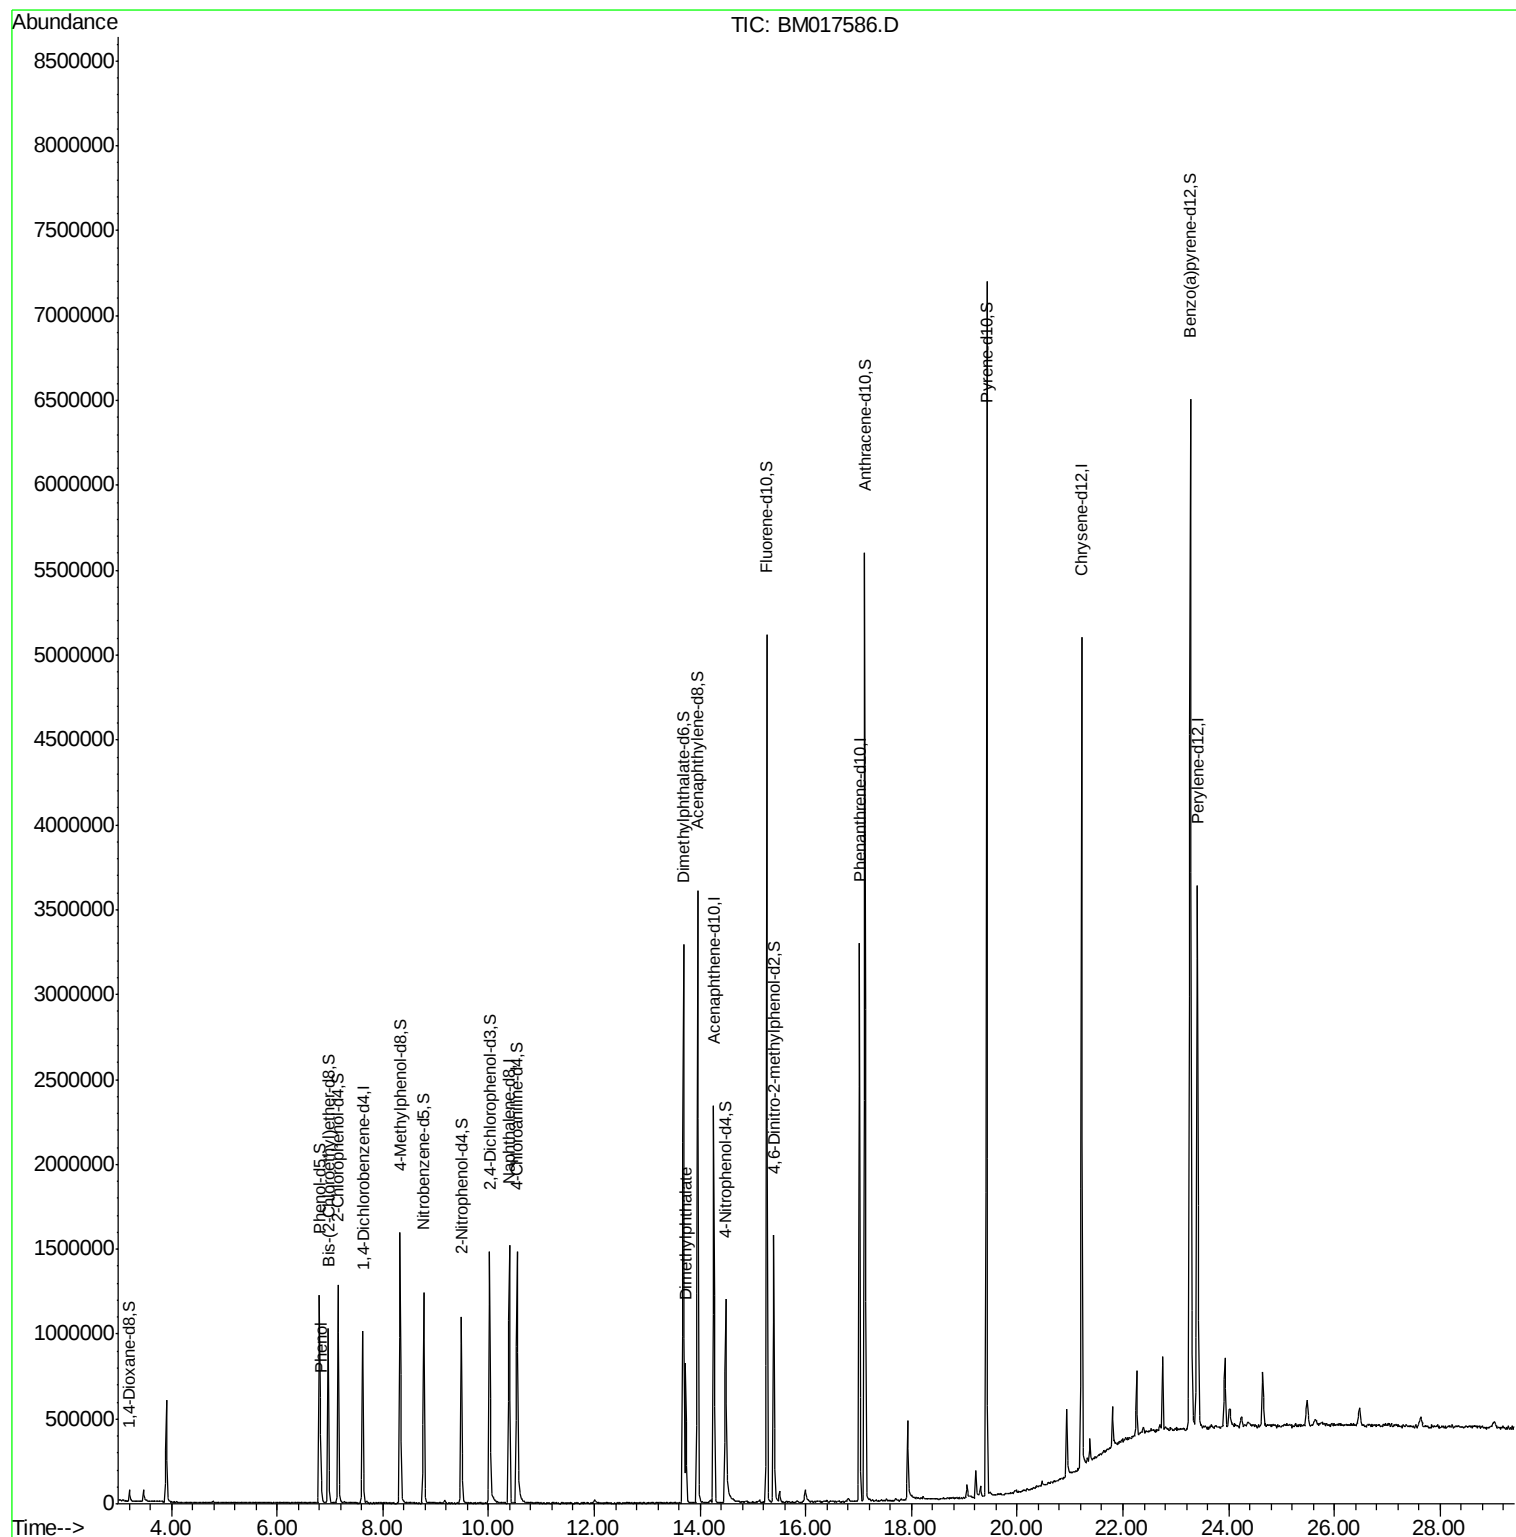

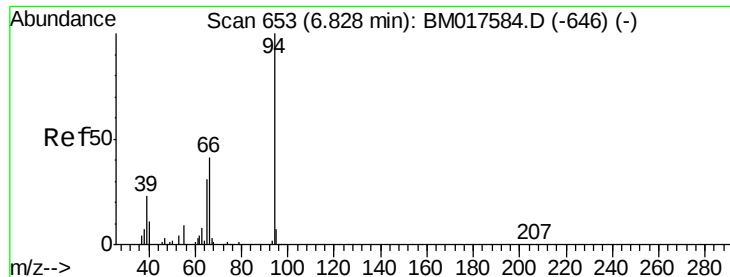

#6

Phenol

Concen: 3.941 ng/ul

RT: 6.83 min Scan# 653

Delta R.T. -0.01 min

Lab File: BM017586.D

Acq: 09 Nov 2018 03:35

Instrument :

BNA_M

ClientSampleId :

ESNS4





Tgt Ion: 94 Resp: 96504

Ion Ratio Lower Upper

94 100

65 31.2 24.0 36.0

66 44.4 31.1 46.7

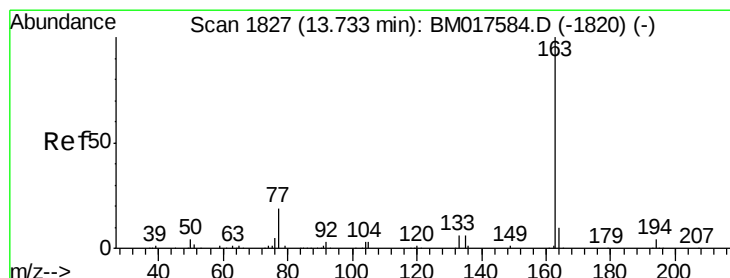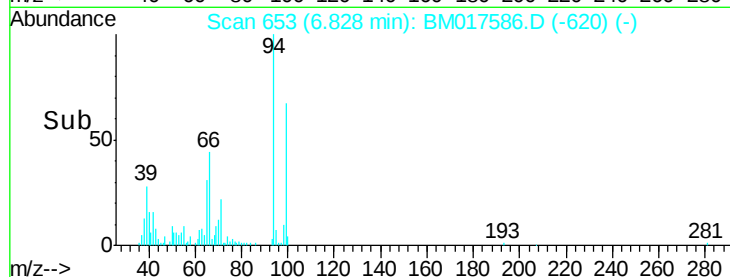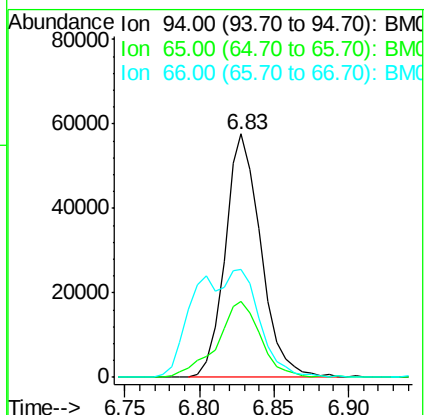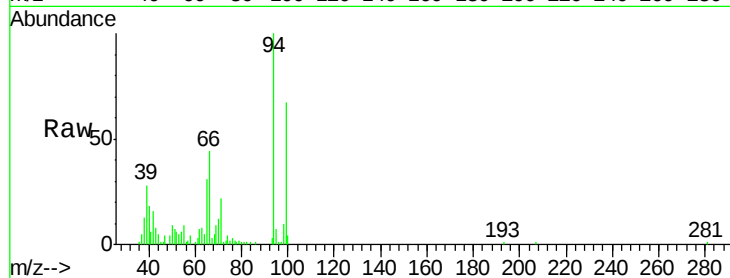

#45

Dimethylphthalate

Concen: 8.440 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BM017586.D

Acq: 09 Nov 2018 03:35

Tgt Ion: 163 Resp: 521414

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.5 8.1 12.1

