
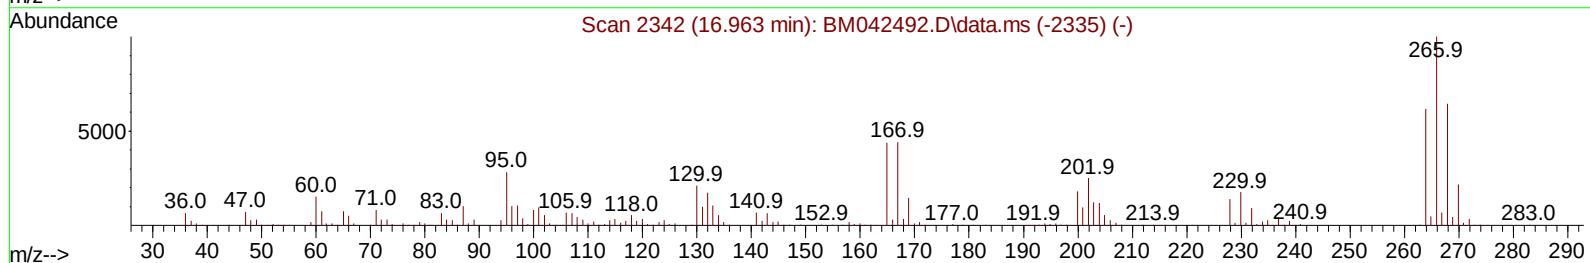
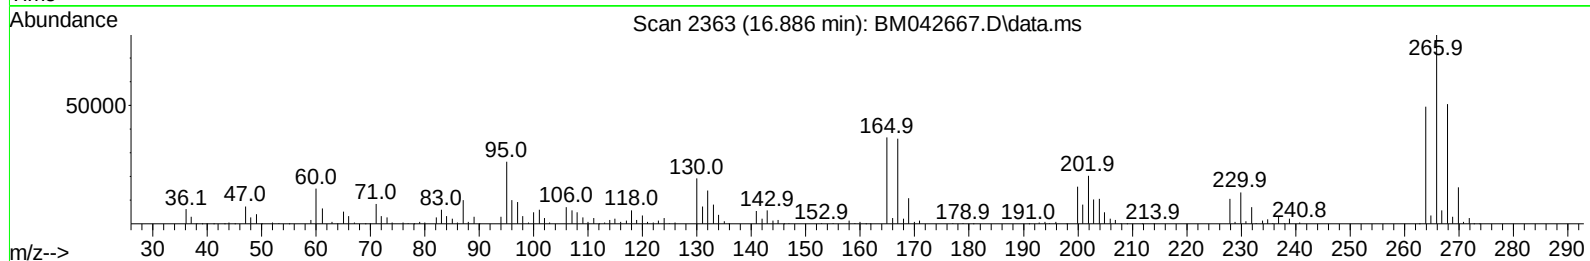


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110923\
Data File : BM042667.D
Acq On : 09 Nov 2023 11:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 19:27:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 13:21:00 2023
Response via : Initial Calibration

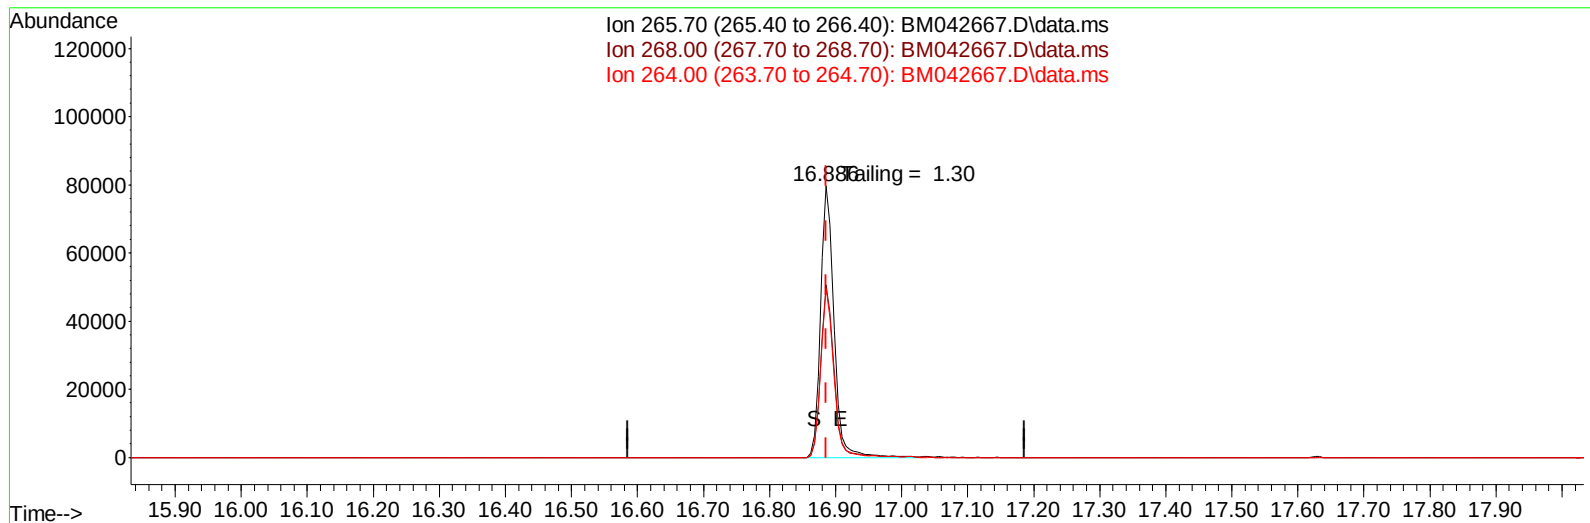

TIC: BM042667.D\data.ms

(70) Pentachlorophenol (C)




16.886min (-0.000) 0.00 ng

response 110876

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.63
264.00	61.80	62.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110923\
Data File : BM042667.D
Acq On : 09 Nov 2023 11:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 09 19:27:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 13:21:00 2023
Response via : Initial Calibration

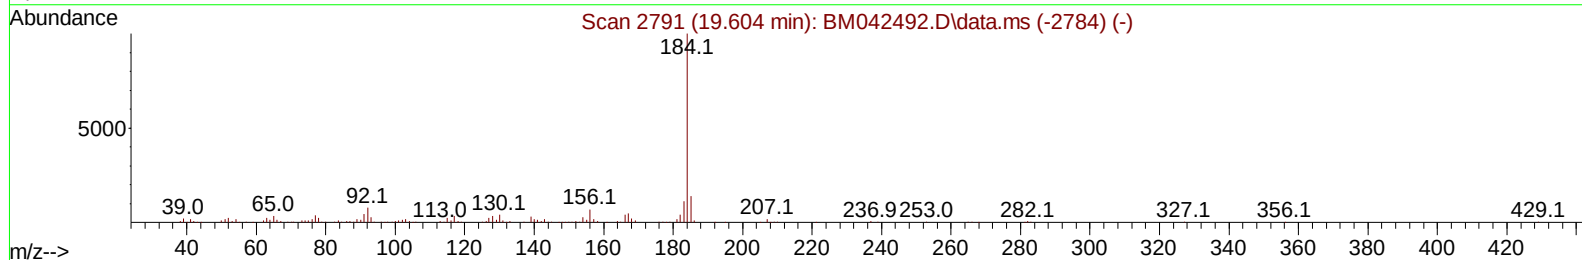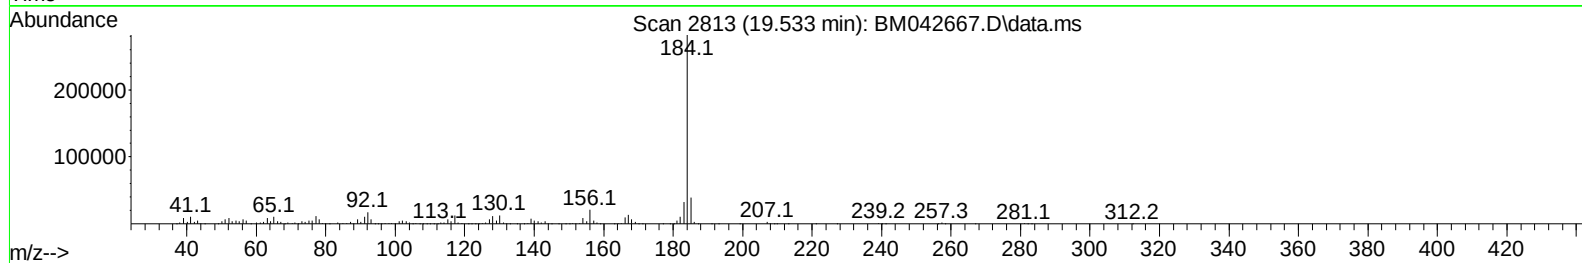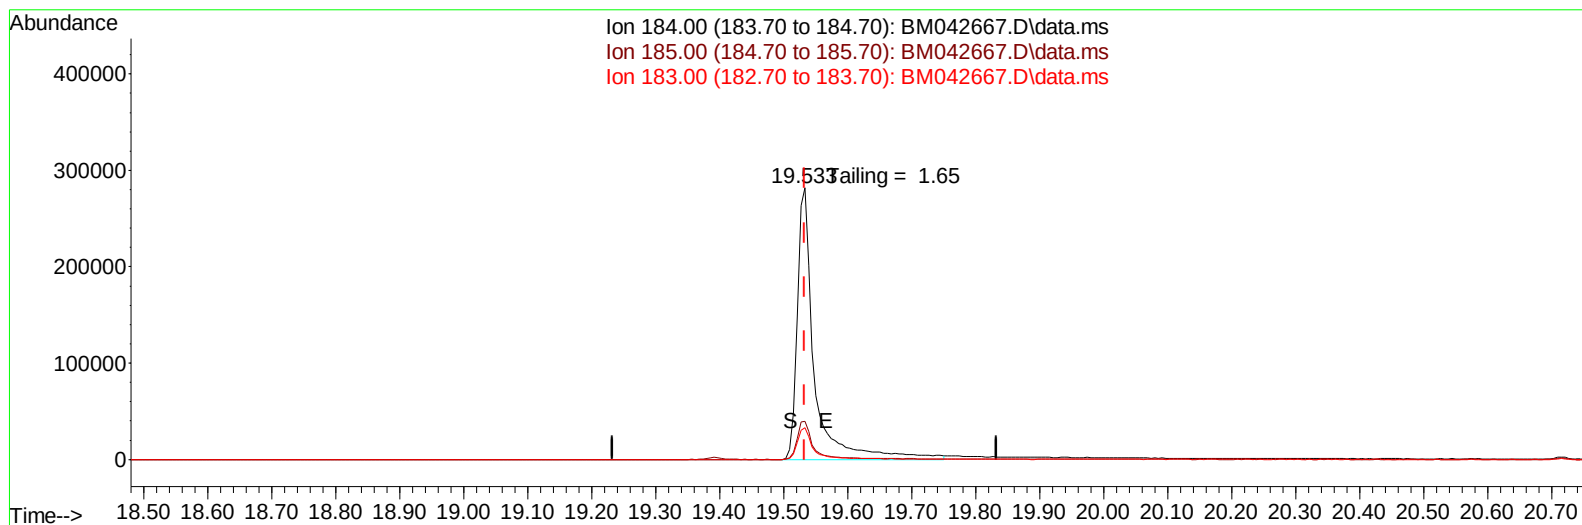

TIC: BM042667.D\data.ms

(77) Benzidine**19.533min (-0.000) 32283.70 ng****response 526756**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.10
183.00	11.20	11.73
0.00	0.00	0.00