

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110923\
 Data File : BM042669.D
 Acq On : 09 Nov 2023 13:15
 Operator : MA/JU
 Sample : PB156951BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB156951BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM042669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.375	400	406	420	rBV	928933	1369480	57.90%	10.438%
2	7.010	677	684	704	rBV	901021	1404005	59.36%	10.701%
3	7.845	820	826	838	rBV	284153	455867	19.27%	3.475%
4	9.045	1022	1030	1043	rBV	499724	840595	35.54%	6.407%
5	10.663	1298	1305	1316	rBV	311903	535793	22.65%	4.084%
6	13.122	1715	1723	1741	rBV	1240043	1712867	72.42%	13.055%
7	14.504	1951	1958	1970	rBV	468135	677403	28.64%	5.163%
8	15.998	2206	2212	2229	rBV	1044845	1401343	59.25%	10.681%
9	17.257	2420	2426	2442	rBV	531311	753088	31.84%	5.740%
10	18.104	2565	2570	2585	rBV	25949	57635	2.44%	0.439%
11	19.386	2785	2788	2797	rBV4	13873	25991	1.10%	0.198%
12	19.874	2865	2871	2882	rBV	2034488	2365121	100.00%	18.027%
13	21.439	3132	3137	3144	rBV	558817	731221	30.92%	5.573%
14	23.815	3534	3541	3554	rBV	373714	789791	33.39%	6.020%




Sum of corrected areas: 13120200

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110923\
Data File : BM042669.D
Acq On : 09 Nov 2023 13:15
Operator : MA/JU
Sample : PB156951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156951BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

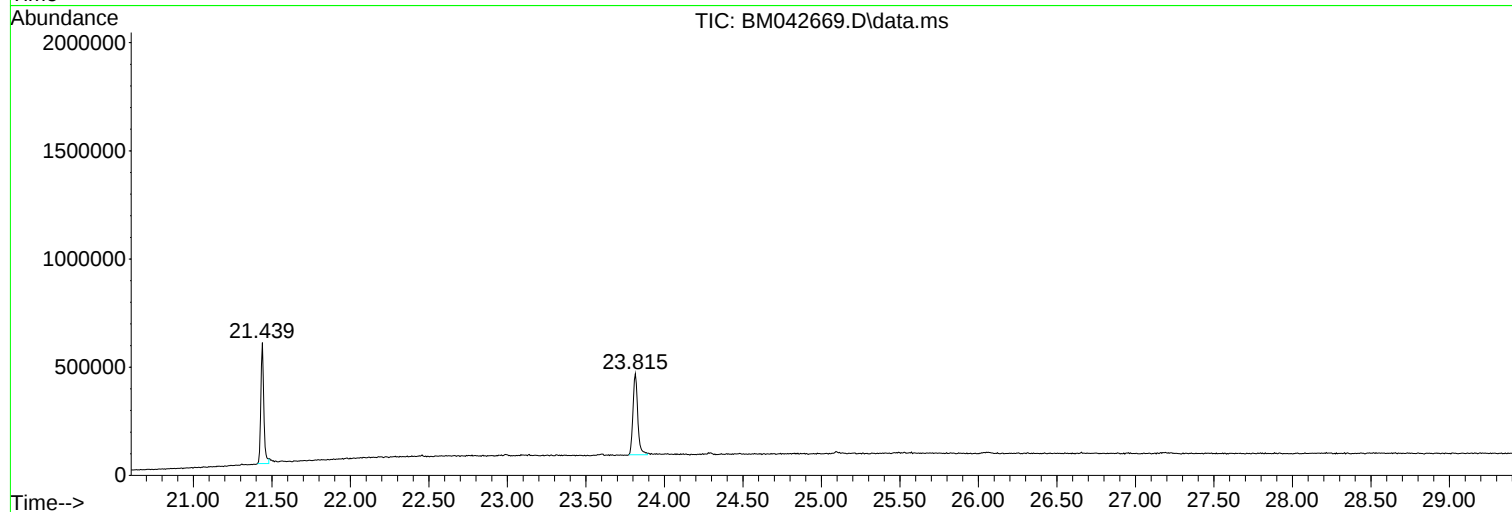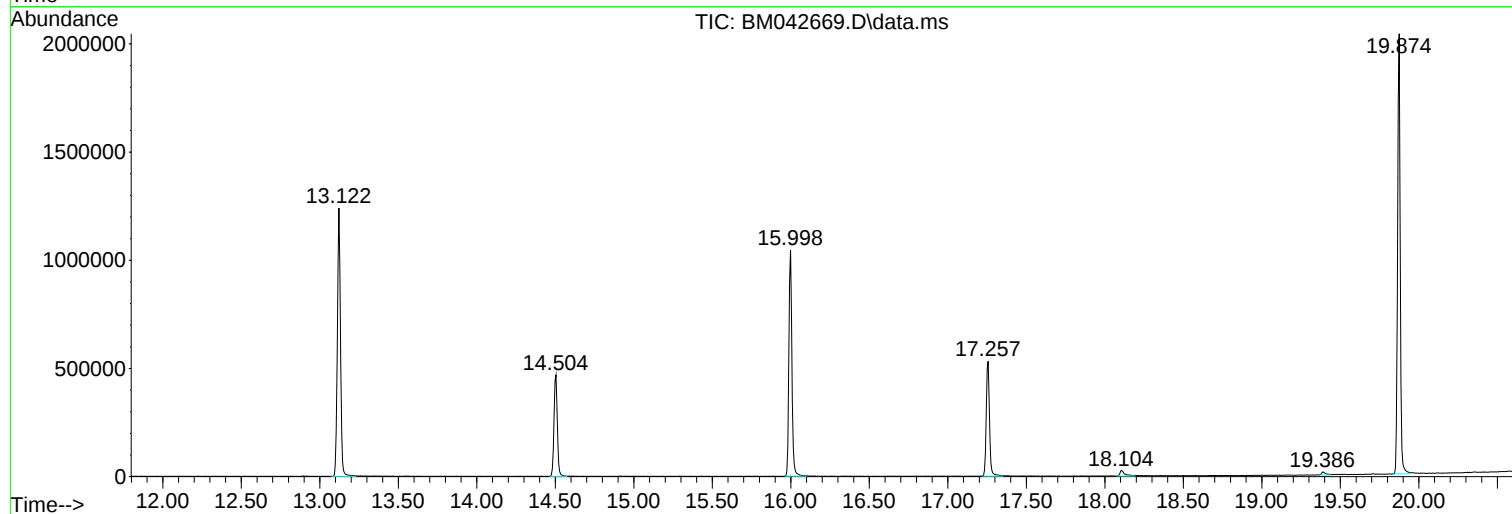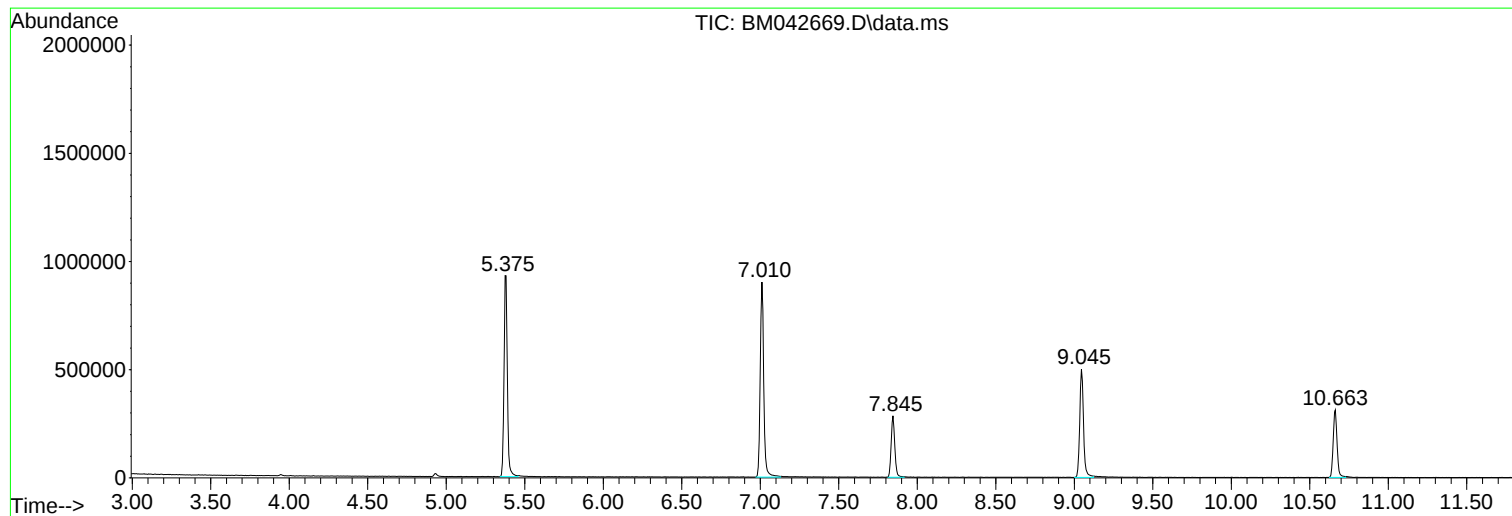

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110923\
Data File : BM042669.D
Acq On : 09 Nov 2023 13:15
Operator : MA/JU
Sample : PB156951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156951BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM110923\
Data File : BM042669.D
Acq On : 09 Nov 2023 13:15
Operator : MA/JU
Sample : PB156951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156951BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------