


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111018\
 Data File : BM017590.D
 Acq On : 09 Nov 2018 14:00
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM101718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 29 15:08:36 2018

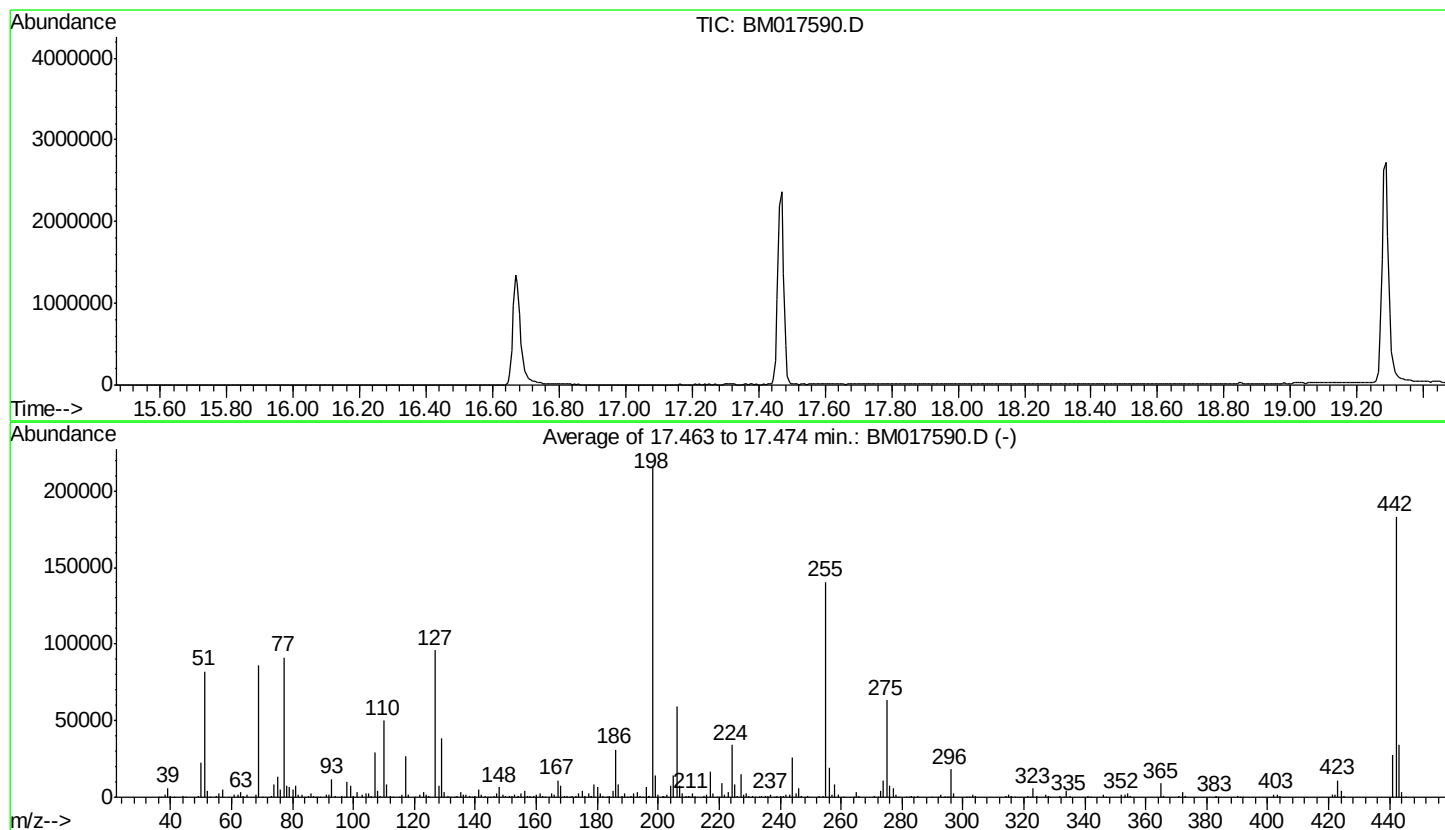

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	82285	PASS
68	69	0.00	2	2.0	1750	PASS
69	198	0.00	100	39.7	85877	PASS
70	69	0.00	2	0.3	226	PASS
127	198	10	80	44.3	95970	PASS
197	198	0.00	2	0.5	1105	PASS
198	198	100	100	100.0	216469	PASS
199	198	5	9	6.6	14387	PASS
275	198	10	60	29.2	63314	PASS
365	198	1	100	4.2	9134	PASS
441	198	0.01	100	12.6	27378	PASS
442	198	50	100	84.7	183445	PASS
443	442	15	24	18.7	34360	PASS