
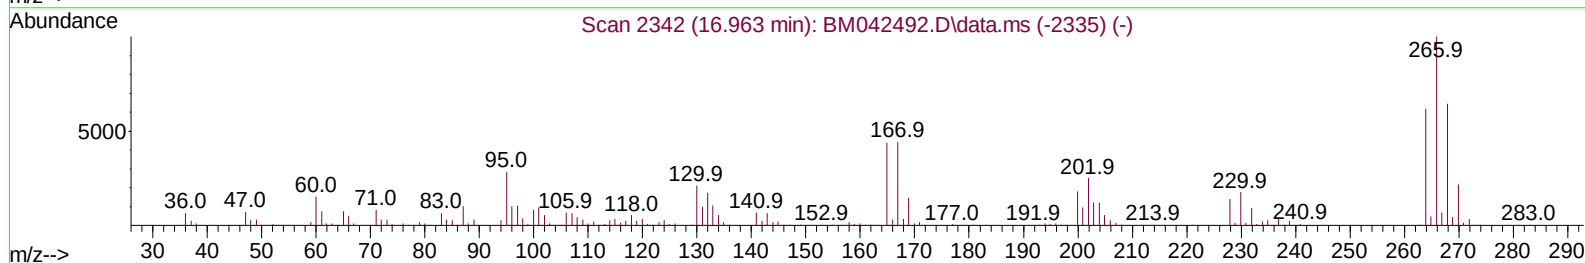
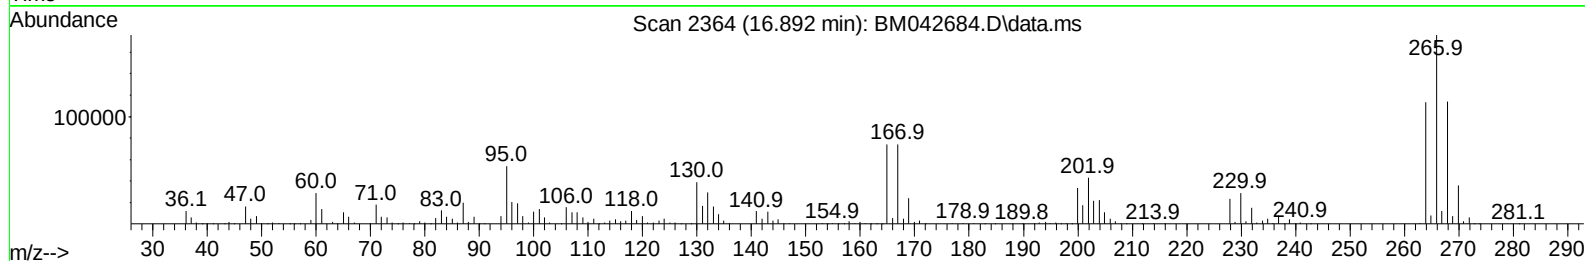


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111023\
Data File : BM042684.D
Acq On : 10 Nov 2023 10:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 23:40:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 13:21:00 2023
Response via : Initial Calibration

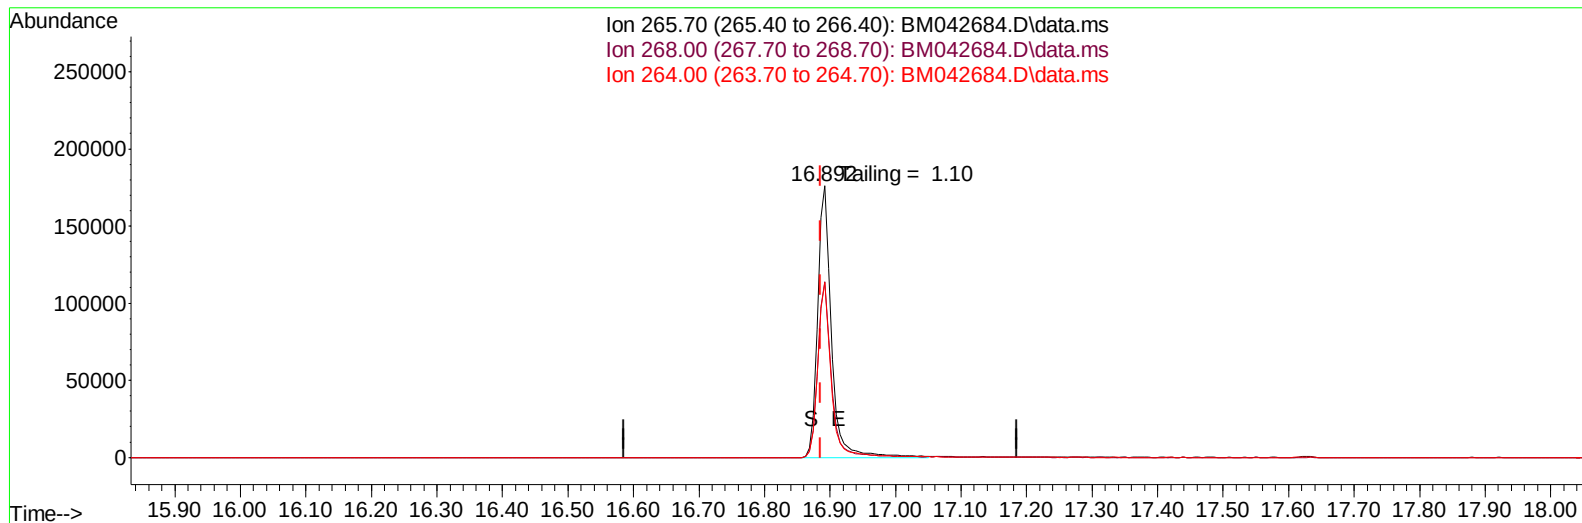




TIC: BM042684.D\data.ms

(70) Pentachlorophenol (C)**16.892min (+ 0.006) 23183.79 ng****response 259063**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.83
264.00	61.80	64.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111023\
Data File : BM042684.D
Acq On : 10 Nov 2023 10:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 10 23:40:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 13:21:00 2023
Response via : Initial Calibration

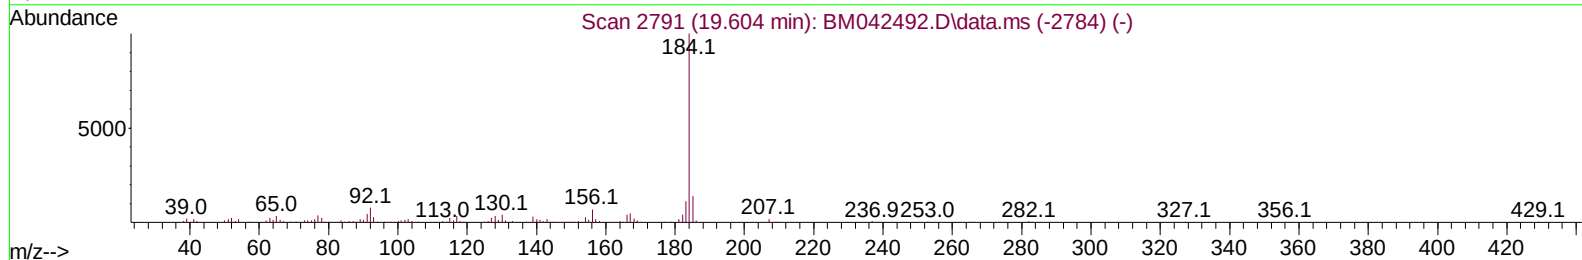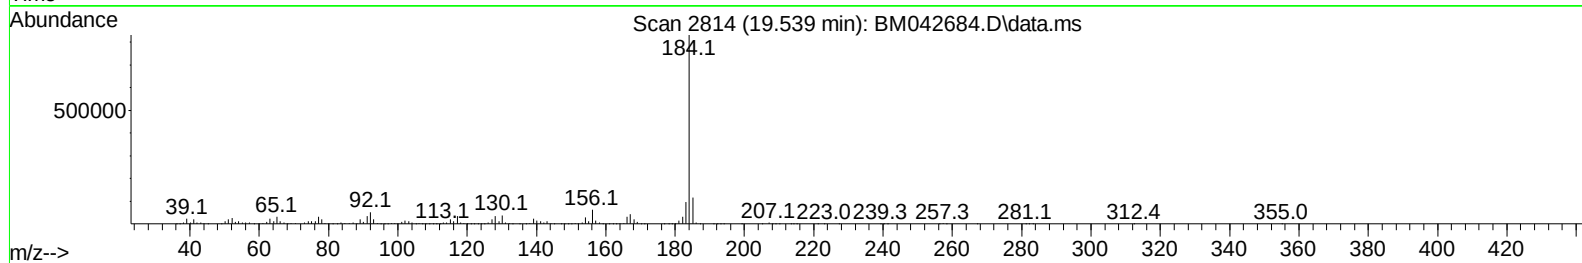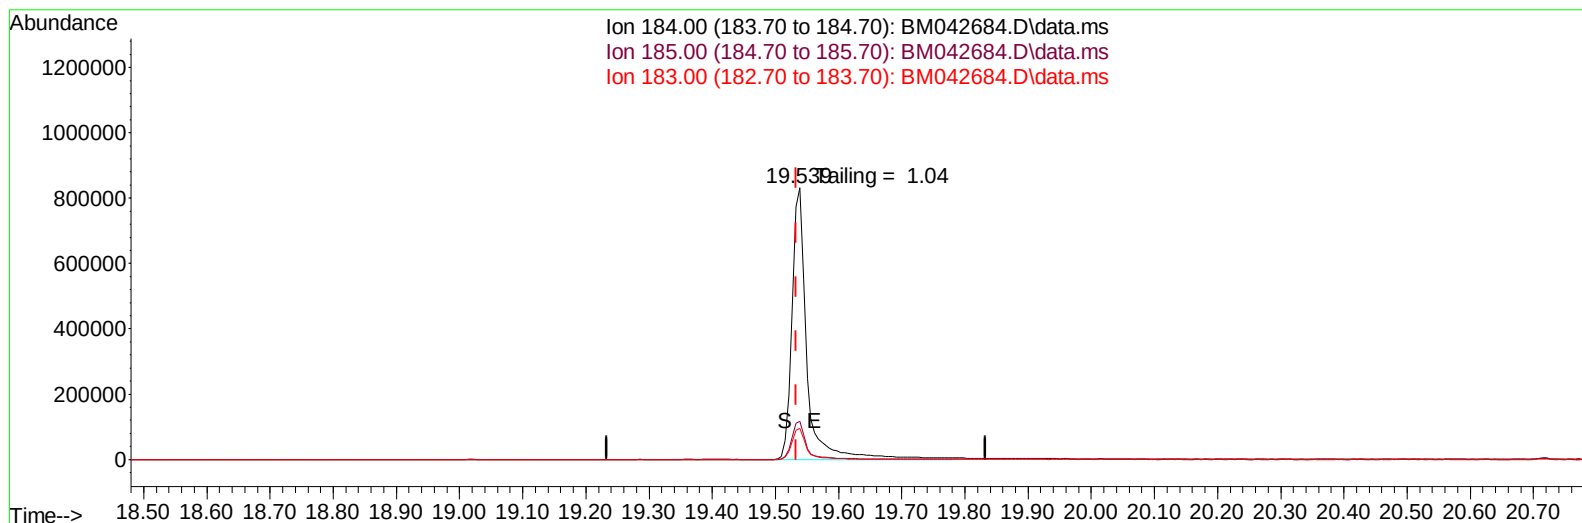

TIC: BM042684.D\data.ms

(77) Benzidine**19.539min (+ 0.006) 32333.73 ng****response 1369641**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.96
183.00	11.20	11.44
0.00	0.00	0.00