

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111023\
 Data File : BM042686.D
 Acq On : 10 Nov 2023 11:58
 Operator : MA/JU
 Sample : PB156988BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB156988BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM042686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	401	407	433	rBV	1346164	1997309	32.73%	9.232%
2	7.016	678	685	705	rBV	1278188	2129577	34.90%	9.843%
3	7.845	820	826	837	rBV	183323	307576	5.04%	1.422%
4	9.051	1022	1031	1050	rBV	744128	1330768	21.81%	6.151%
5	10.663	1297	1305	1316	rBV	219961	397786	6.52%	1.839%
6	13.121	1717	1723	1747	rBV	2219095	3241472	53.12%	14.982%
7	14.504	1952	1958	1970	rBV	392131	588230	9.64%	2.719%
8	15.998	2206	2212	2233	rBV	2150191	3077392	50.43%	14.224%
9	17.256	2419	2426	2442	rBV	474327	738309	12.10%	3.413%
10	19.874	2865	2871	2888	rBV	5139644	6101772	100.00%	28.203%
11	21.439	3132	3137	3150	rBV	596587	896188	14.69%	4.142%
12	23.815	3535	3541	3560	rVB	356440	828695	13.58%	3.830%




Sum of corrected areas: 21635074

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111023\
Data File : BM042686.D
Acq On : 10 Nov 2023 11:58
Operator : MA/JU
Sample : PB156988BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156988BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

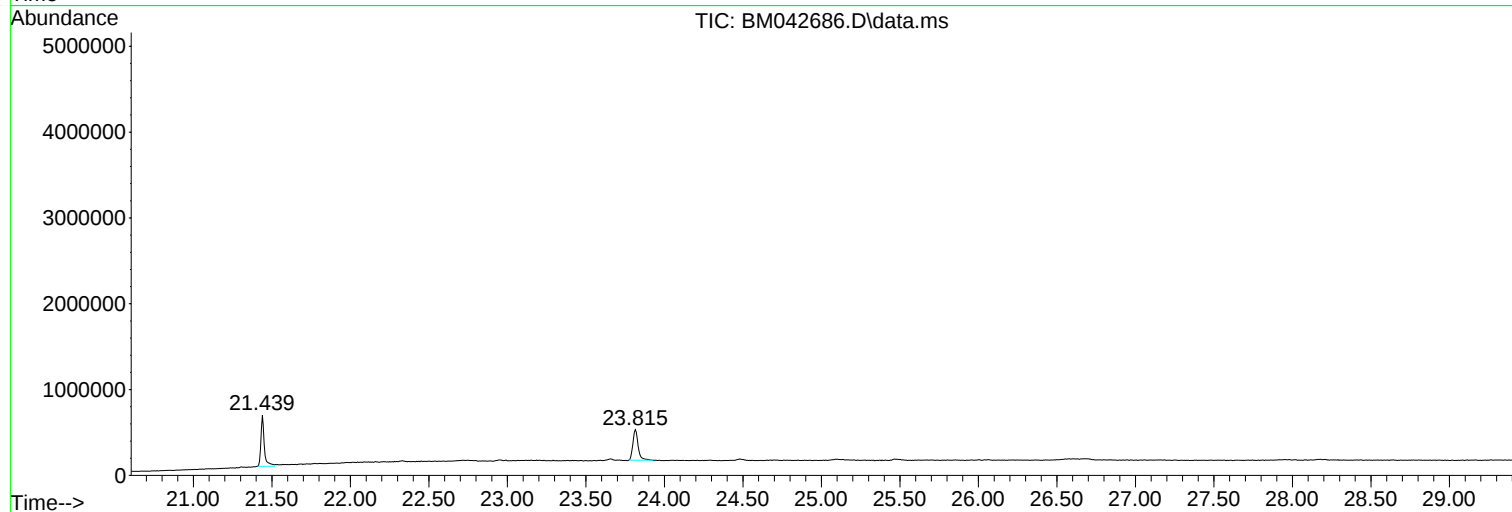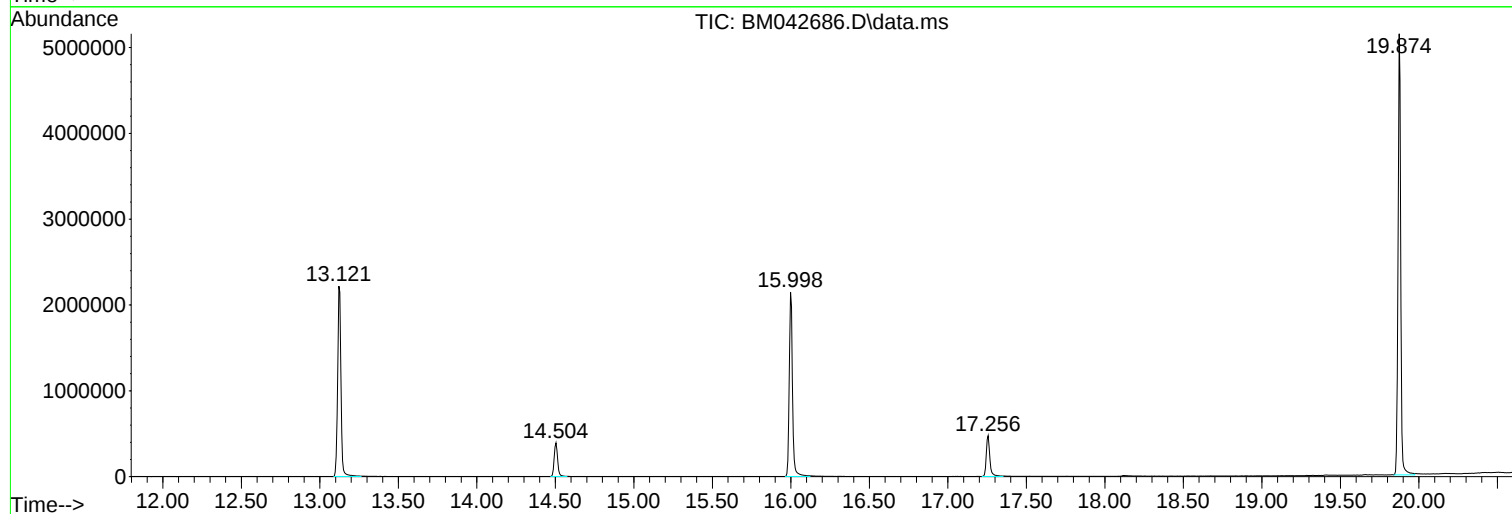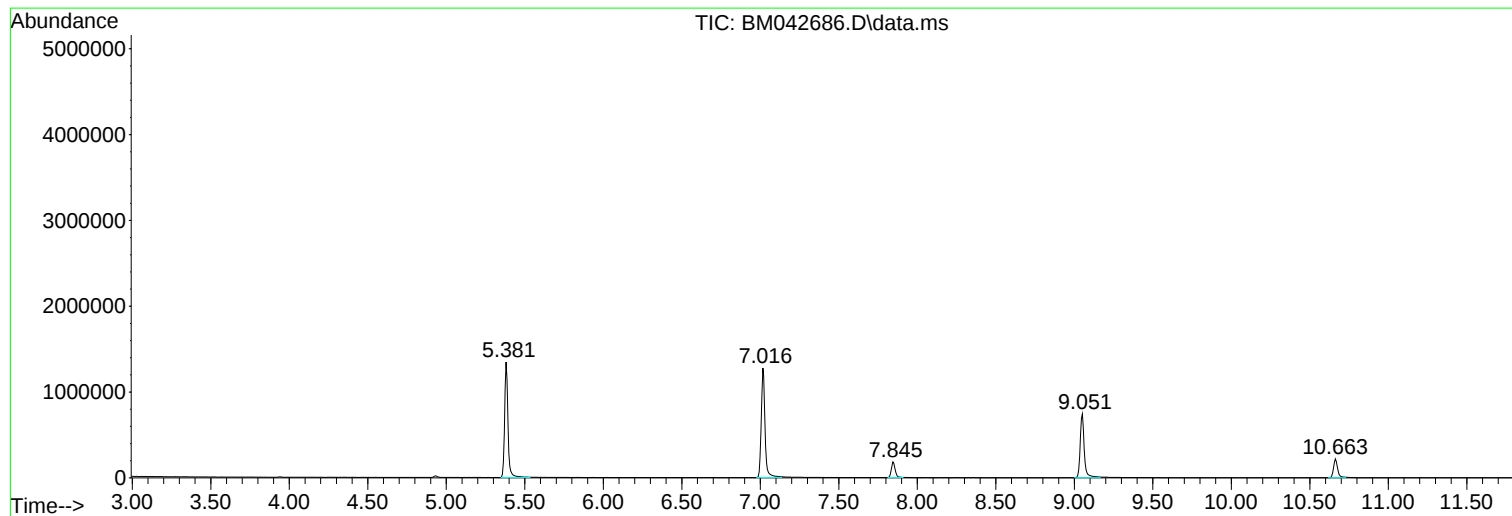

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111023\
Data File : BM042686.D
Acq On : 10 Nov 2023 11:58
Operator : MA/JU
Sample : PB156988BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156988BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111023\
Data File : BM042686.D
Acq On : 10 Nov 2023 11:58
Operator : MA/JU
Sample : PB156988BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB156988BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------