


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111023\
Data File : BM042684.D
Acq On : 10 Nov 2023 10:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 09 13:21:00 2023

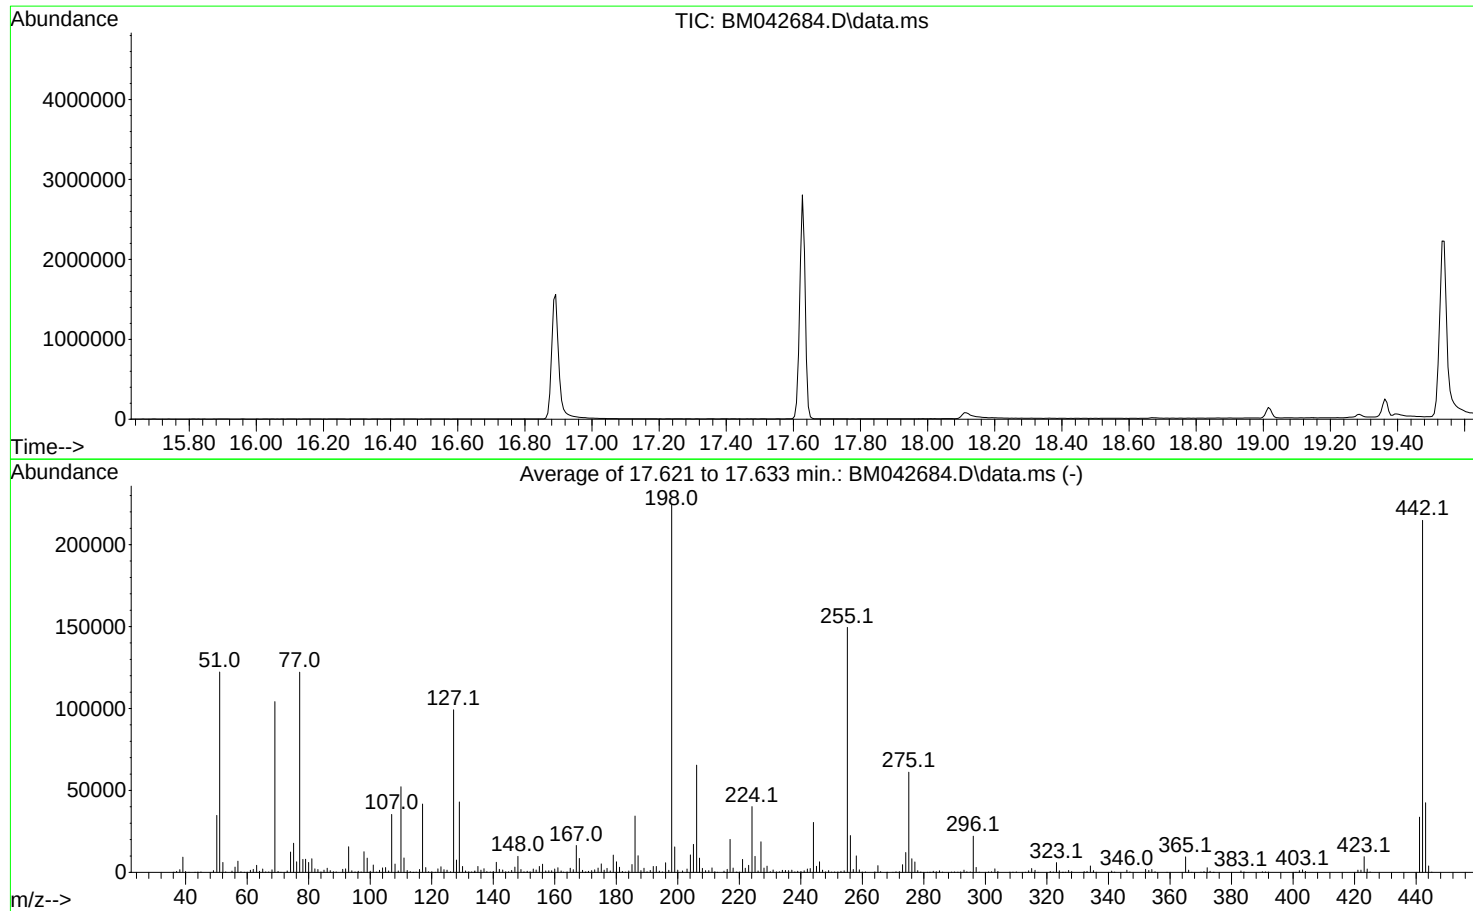




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	122316	PASS
68	69	0.00	2	1.5	1590	PASS
69	198	0.00	100	46.4	104171	PASS
70	69	0.00	2	0.6	600	PASS
127	198	10	80	44.2	99245	PASS
197	198	0.00	2	0.6	1259	PASS
198	198	100	100	100.0	224512	PASS
199	198	5	9	6.9	15509	PASS
275	198	10	60	27.2	61112	PASS
365	198	1	100	4.2	9491	PASS
441	198	0.01	100	15.0	33677	PASS
442	442	50	100	100.0	214848	PASS
443	442	15	24	19.8	42443	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111023\
Data File : BM042684.D
Acq On : 10 Nov 2023 10:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 10 23:40:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 13:21:00 2023
Response via : Initial Calibration

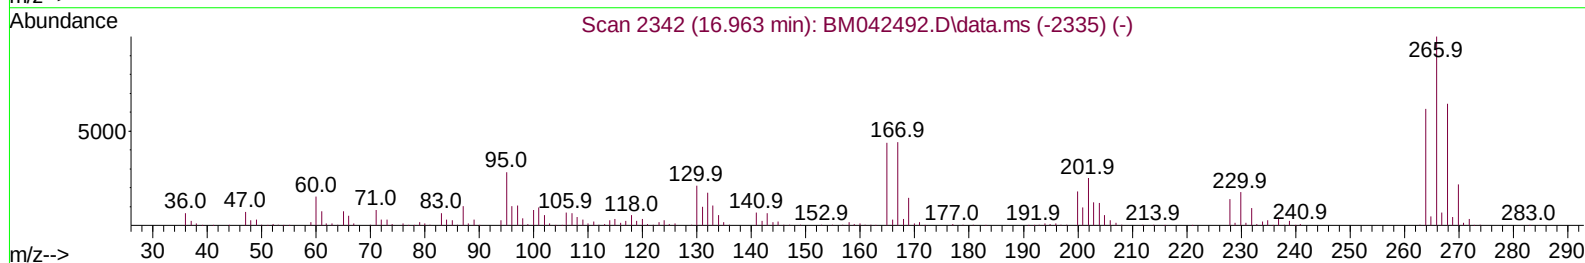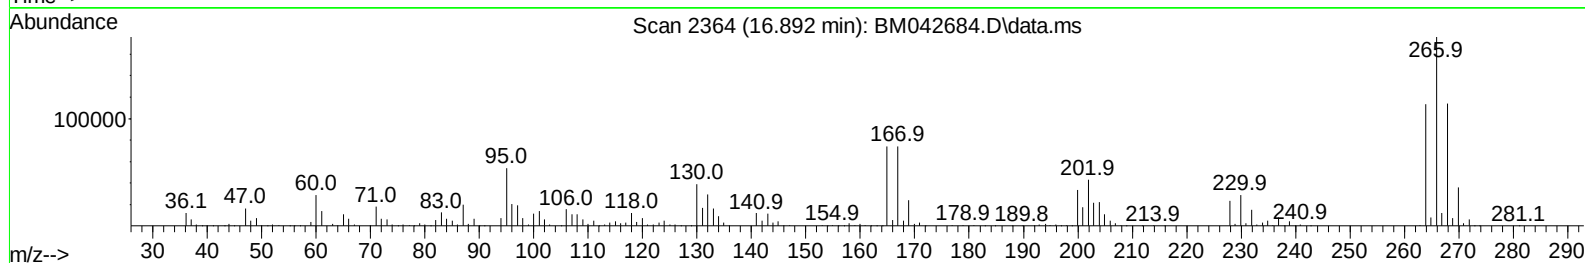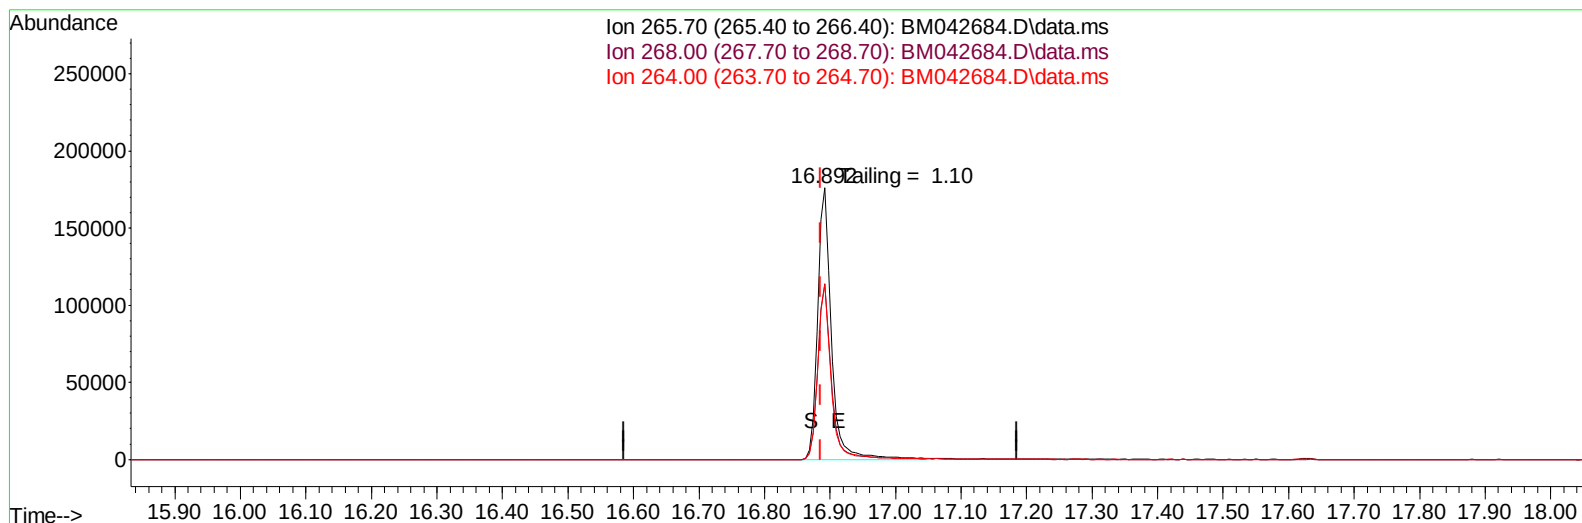

TIC: BM042684.D\data.ms

(70) Pentachlorophenol (C)

16.892min (+ 0.006) 23183.79 ng




response 259063

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.83
264.00	61.80	64.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111023\
Data File : BM042684.D
Acq On : 10 Nov 2023 10:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Nov 10 23:40:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 09 13:21:00 2023
Response via : Initial Calibration

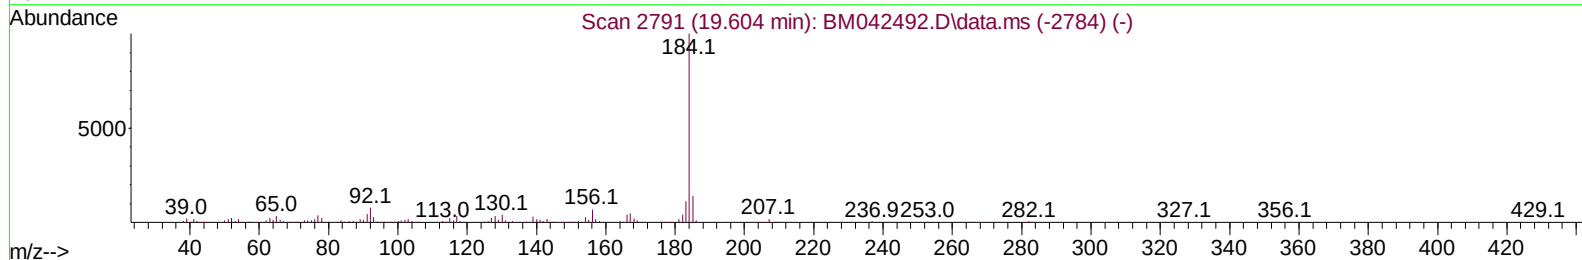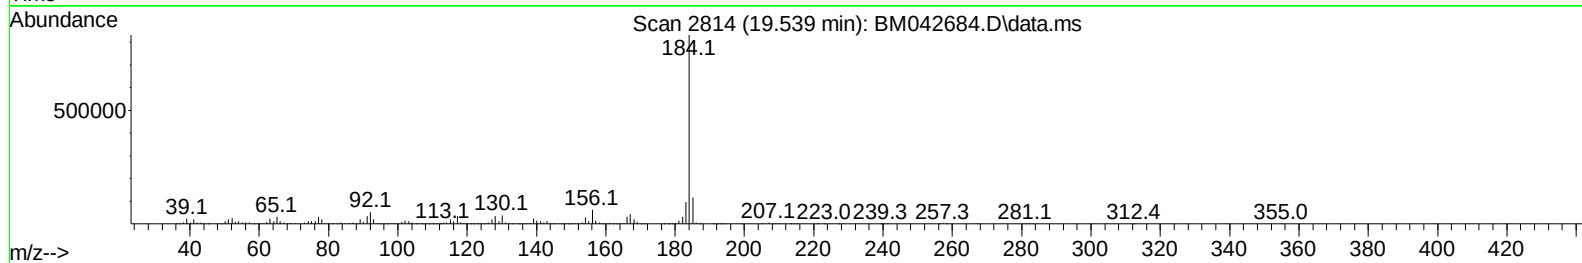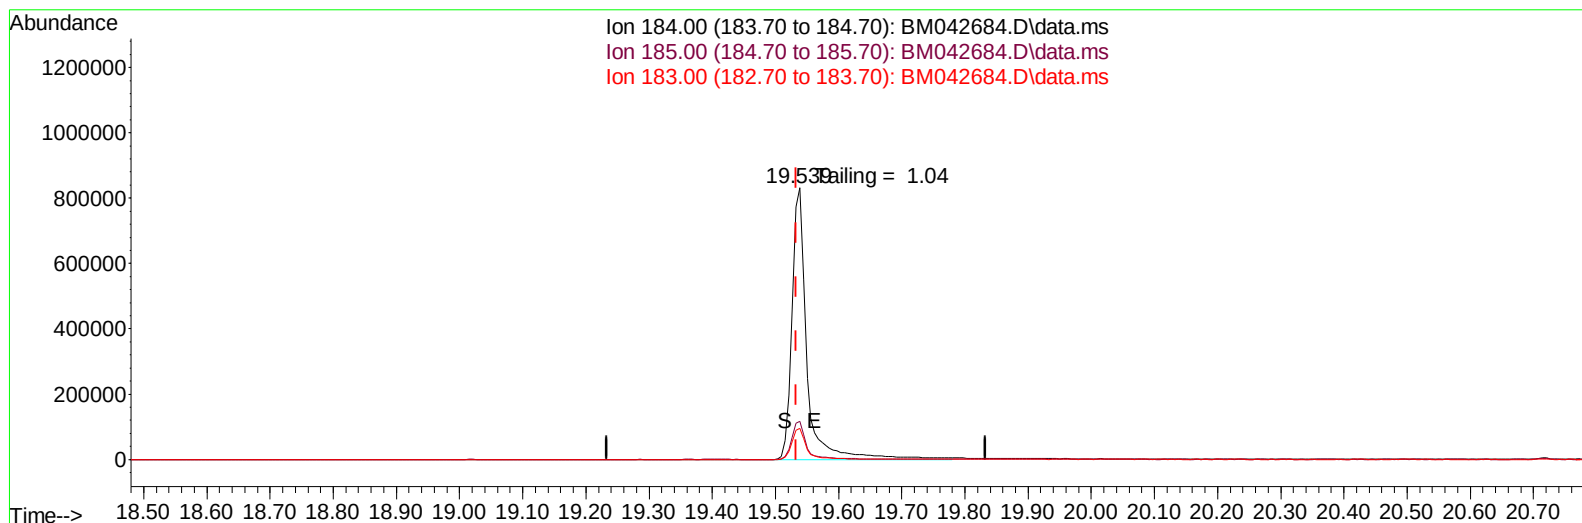

TIC: BM042684.D\data.ms

(77) Benzidine

19.539min (+ 0.006) 32333.73 ng

response 1369641

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.96
183.00	11.20	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/10/2023	BNA_M	<u>BM042684.D</u>
Compound Name	Response	Retention Time
DDT	908521	20.715
DDD	25750	20.28
DDE	359	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26109	934630	2.79

Instrument :
BNA_M
ClientSampleId :
DFTPP