

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111119\
 Data File : BM023638.D
 Acq On : 11 Nov 2019 16:05
 Operator : JU
 Sample : K5535-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEK25

Quant Time: Nov 11 16:45:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 11 16:39:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	362027	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1599847	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1141254	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	2665637	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	2818139	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	3070023	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	22665	2.58	ng/uL	0.00
5) Phenol-d5	6.73	99	440996	13.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	285558	15.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	341863	14.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	361611	13.74	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	163495	14.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	173155	14.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	372942	13.59	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	460676	15.29	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	1432180	16.09	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1541258	15.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	155450	10.23	ng/ul	0.00
58) Fluorene-d10	15.20	176	1264261	16.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	120754	7.83	ng/ul	0.00
71) Anthracene-d10	17.05	188	2090053	16.53	ng/ul	0.00
79) Pyrene-d10	19.35	212	2707427	18.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	3014051	18.66	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	490219	5.621	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111119\
Data File : BM023638.D
Acq On : 11 Nov 2019 16:05
Operator : JU
Sample : K5535-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEK25

Quant Time: Nov 11 16:45:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 11 16:39:45 2019
Response via : Initial Calibration

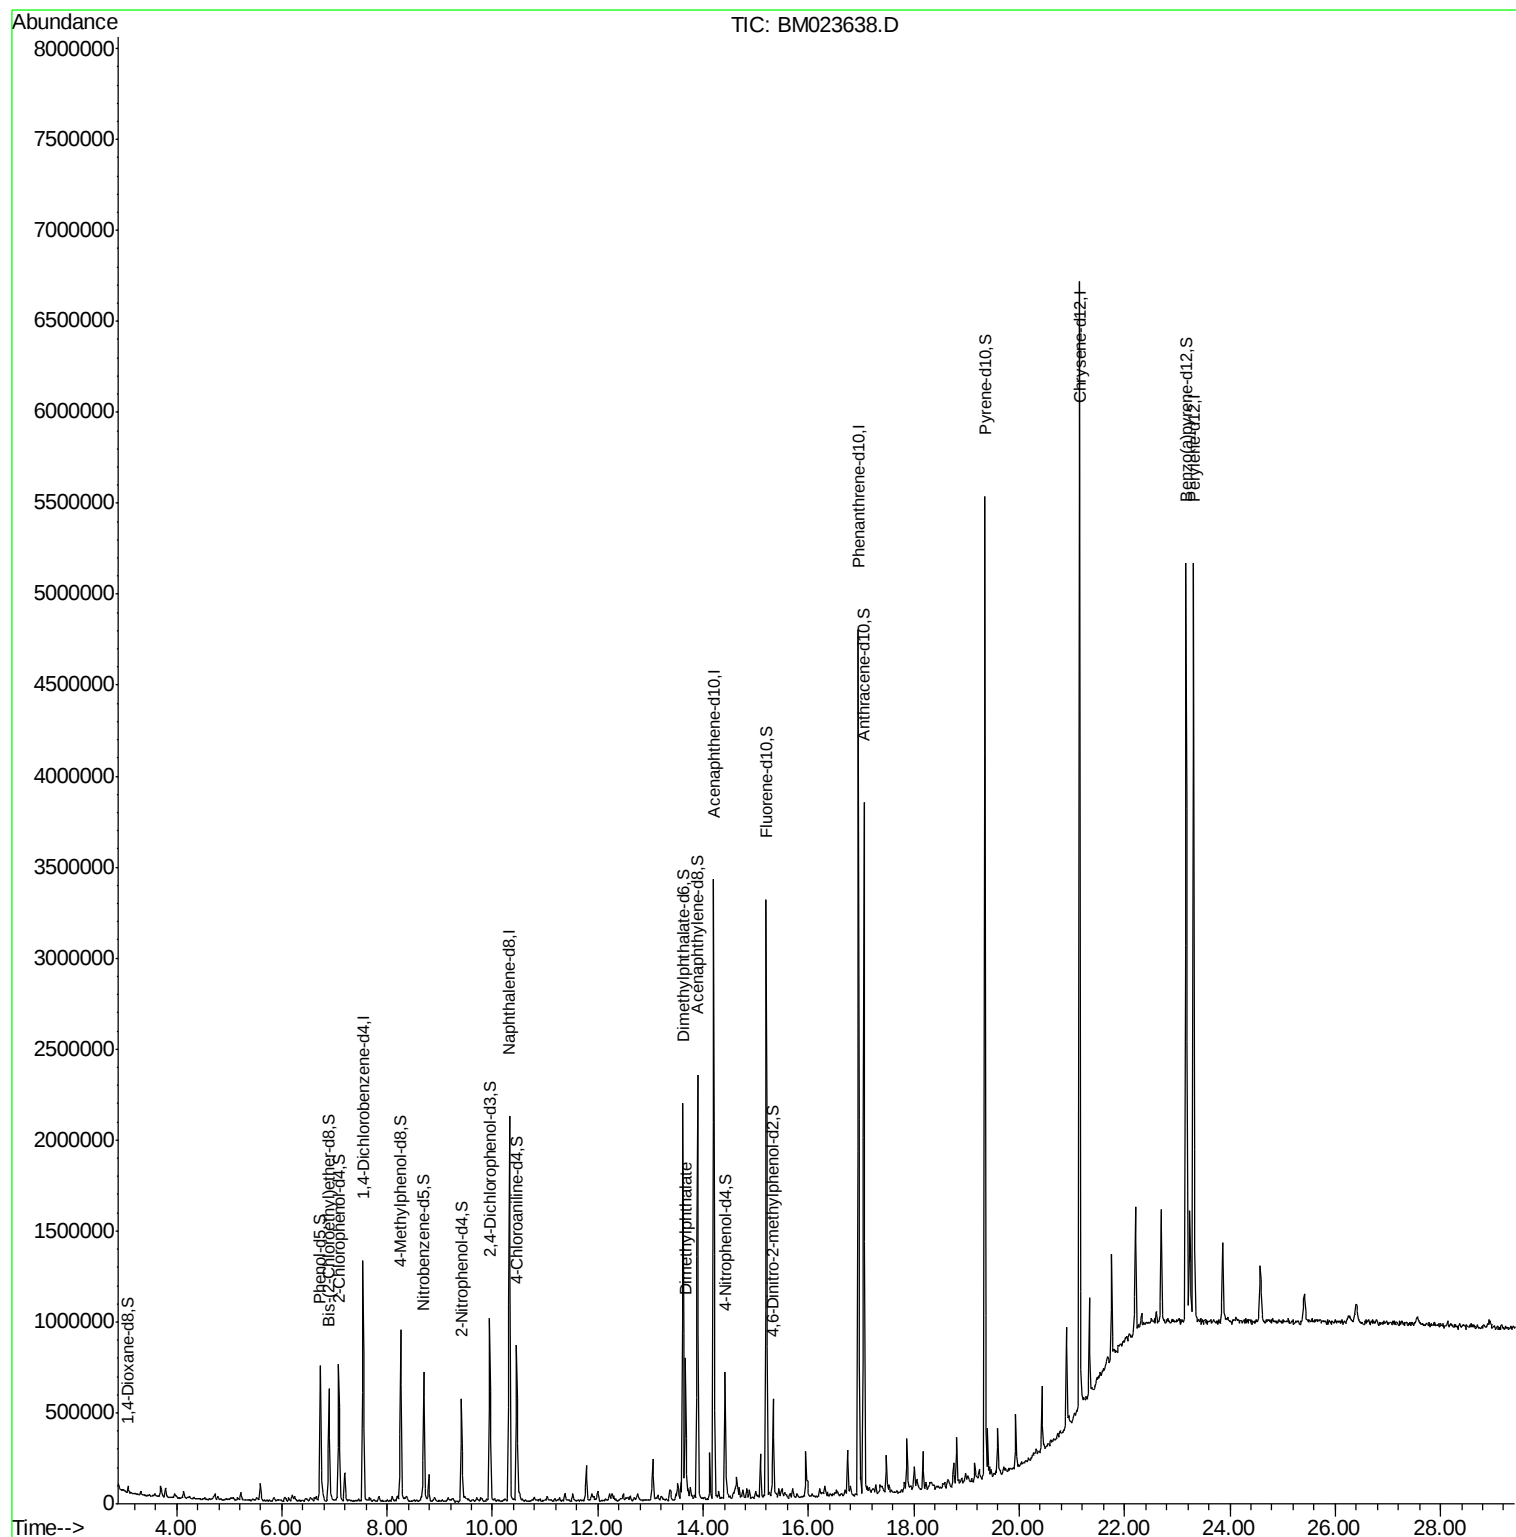

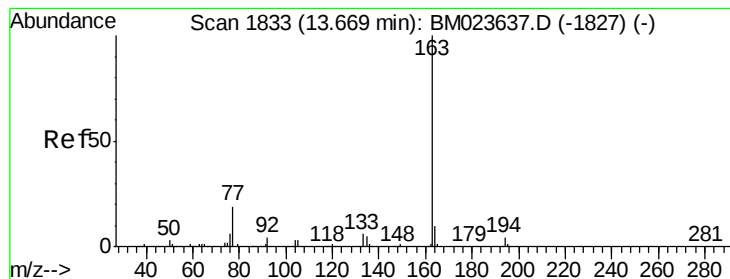

#45

Dimethylphthalate

Concen: 5.621 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: BM023638.D

Acq: 11 Nov 2019 16:05

Instrument :

BNA_M

ClientSampleId :

BEK25


Tot Ion:163 Resp: 490219

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 10.0 8.0 12.0


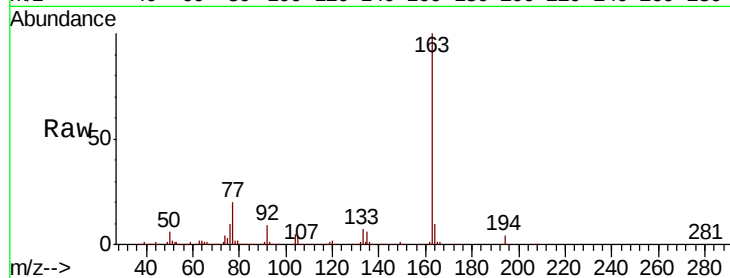


Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

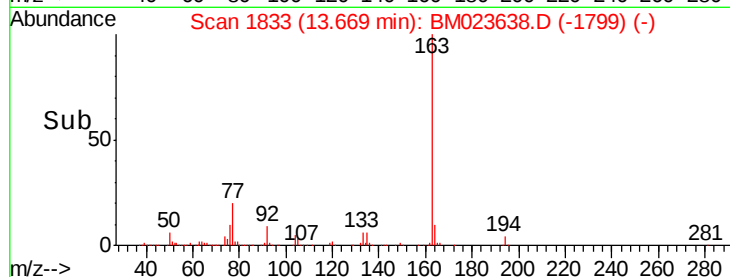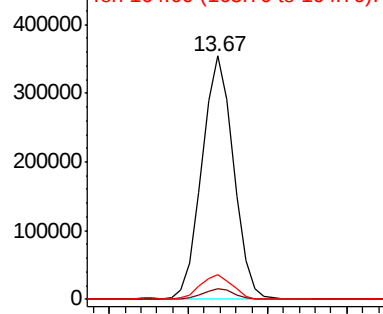

Time-->