

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111119\
 Data File : BM023650.D
 Acq On : 11 Nov 2019 23:17
 Operator : JU
 Sample : K5559-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CQ0

Quant Time: Nov 12 00:06:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 00:02:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	343931	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1594106	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1181892	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	2714419	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	2674695	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	2574117	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	47272	5.67	ng/uL	0.00
5) Phenol-d5	6.73	99	218985	6.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	609635	33.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	641477	28.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	439372	17.57	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	421896	36.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	487005	40.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	888408	32.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	72519	2.41	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	3408844	36.98	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	3890737	36.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	91318	5.80	ng/ul	0.00
58) Fluorene-d10	15.20	176	3045383	37.42	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	548182	34.91	ng/ul	0.00
71) Anthracene-d10	17.05	188	5289184	41.08	ng/ul	0.00
79) Pyrene-d10	19.36	212	6032485	43.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.18	264	5666053	41.83	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	331252	3.667	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111119\
Data File : BM023650.D
Acq On : 11 Nov 2019 23:17
Operator : JU
Sample : K5559-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CQ0

Quant Time: Nov 12 00:06:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 00:02:36 2019
Response via : Initial Calibration

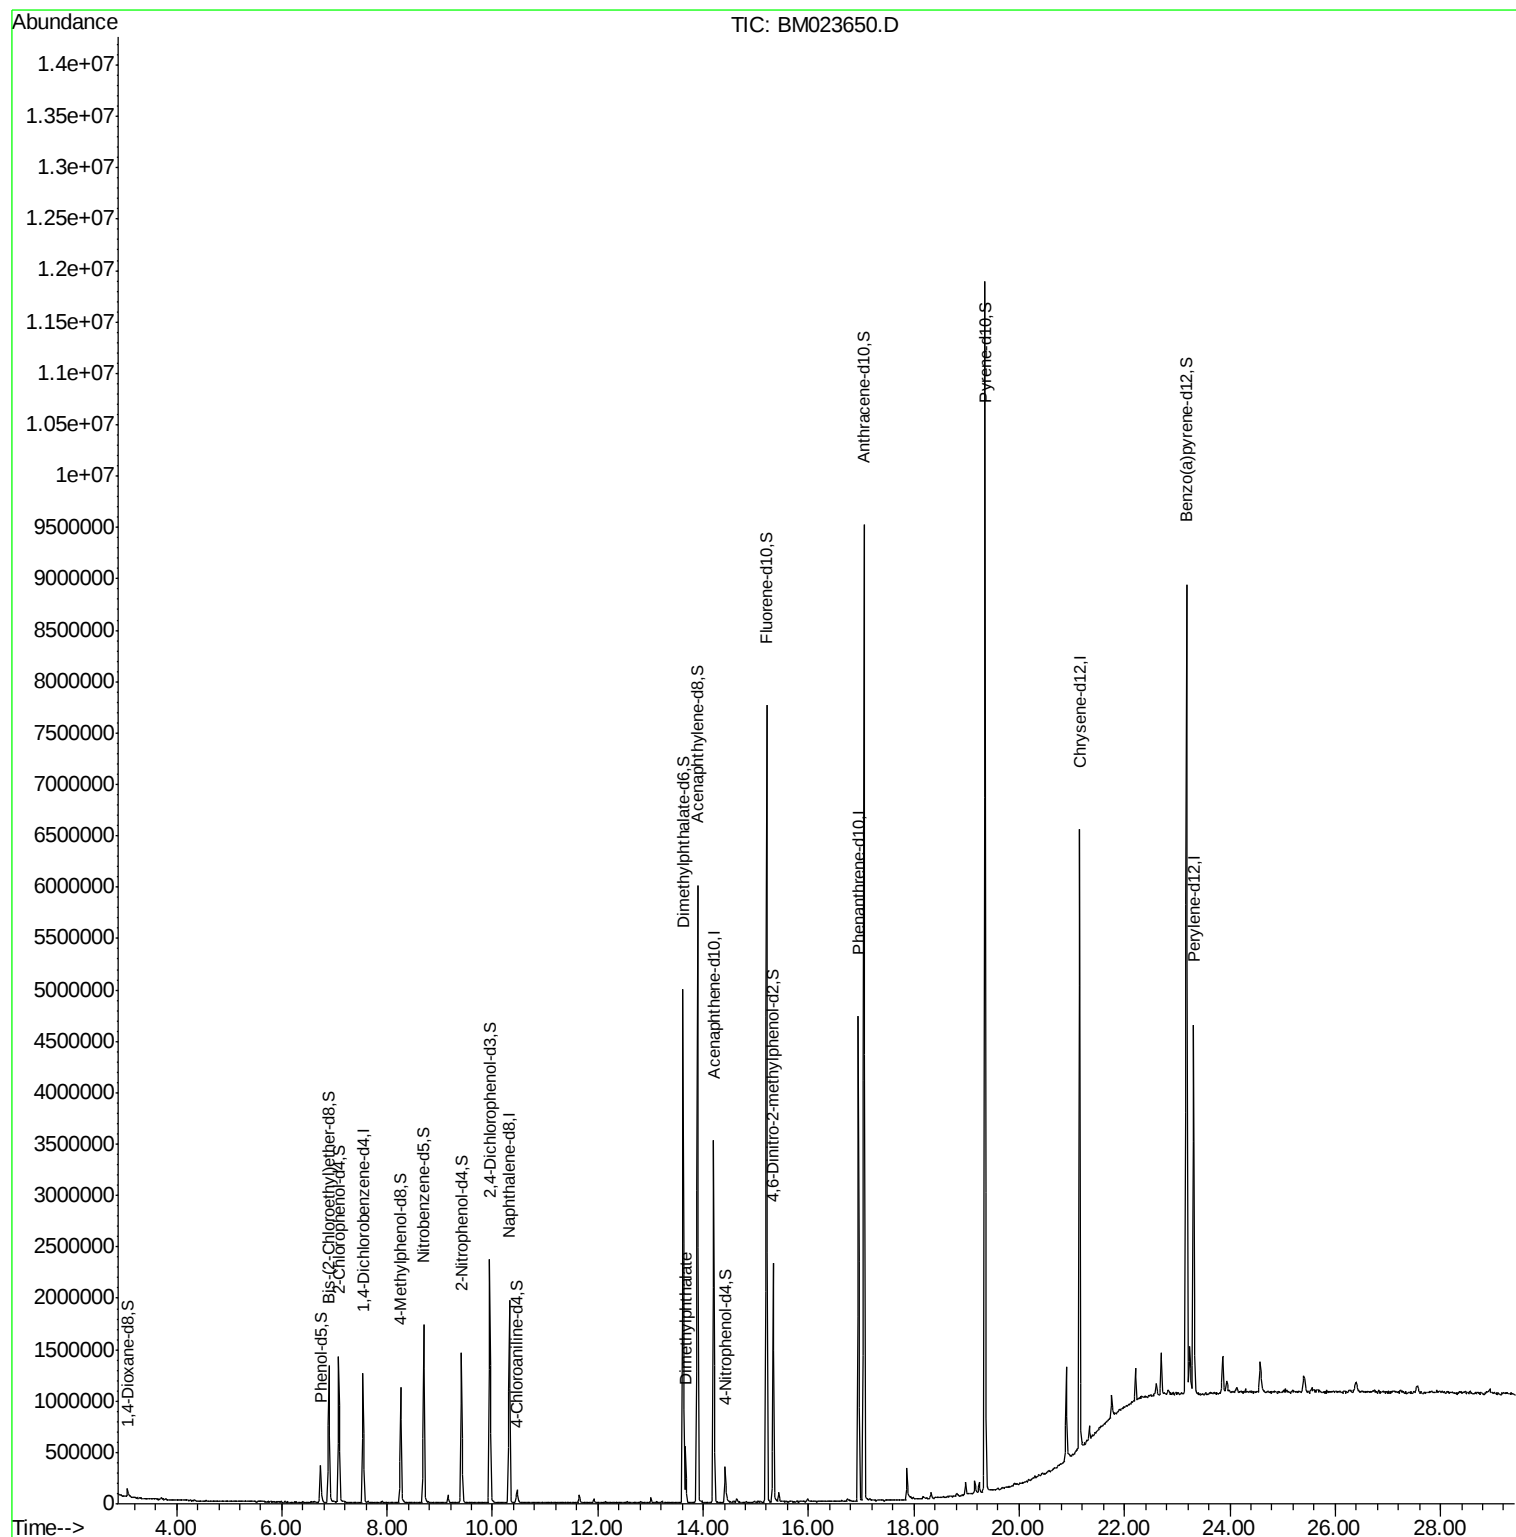

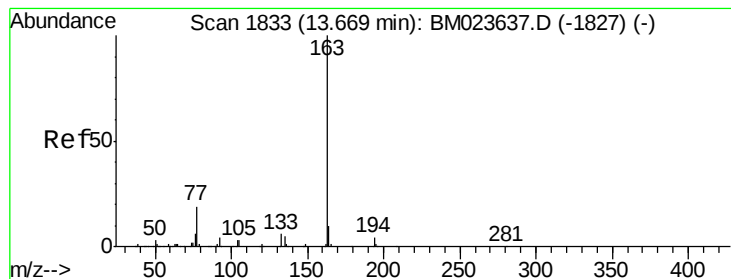

#45

Dimethylphthalate

Concen: 3.667 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: BM023650.D

Acq: 11 Nov 2019 23:17

Instrument :

BNA_M

ClientSampleId :

C0CQ0


Tot Ion:163 Resp: 331252

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.3 8.0 12.0

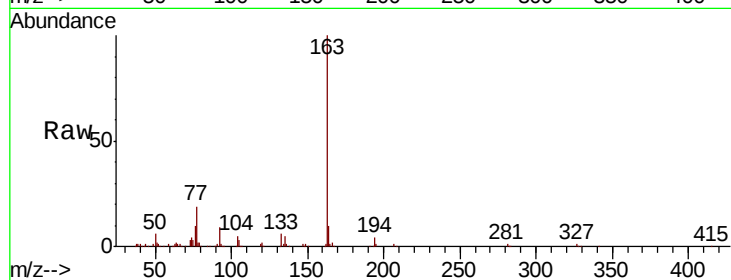

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

