

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111119\
 Data File : BM023651.D
 Acq On : 11 Nov 2019 23:52
 Operator : JU
 Sample : K5559-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CQ1

Quant Time: Nov 12 01:29:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 12 00:02:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	382373	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1751177	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1288597	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	2954222	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	2708965	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	2502615	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	44039	4.75	ng/uL	0.00
5) Phenol-d5	6.73	99	66657	1.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	178915	8.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	184962	7.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	138060	4.97	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	115664	9.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	126726	9.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	261980	8.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	25646	0.78	ng/ul	0.01
44) Dimethylphthalate-d6	13.62	166	1208151	12.02	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1194357	10.41	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	20312	1.18	ng/ul	0.00
58) Fluorene-d10	15.20	176	1039094	11.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	131508	7.70	ng/ul	0.00
71) Anthracene-d10	17.05	188	1990667	14.20	ng/ul	0.00
79) Pyrene-d10	19.35	212	2256784	15.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	1958624	14.87	ng/ul	-0.01

Target Compounds


					Ovalue	
45) Dimethylphthalate	13.67	163	141444	1.436	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111119\
Data File : BM023651.D
Acq On : 11 Nov 2019 23:52
Operator : JU
Sample : K5559-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CQ1

Quant Time: Nov 12 01:29:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 12 00:02:36 2019
Response via : Initial Calibration

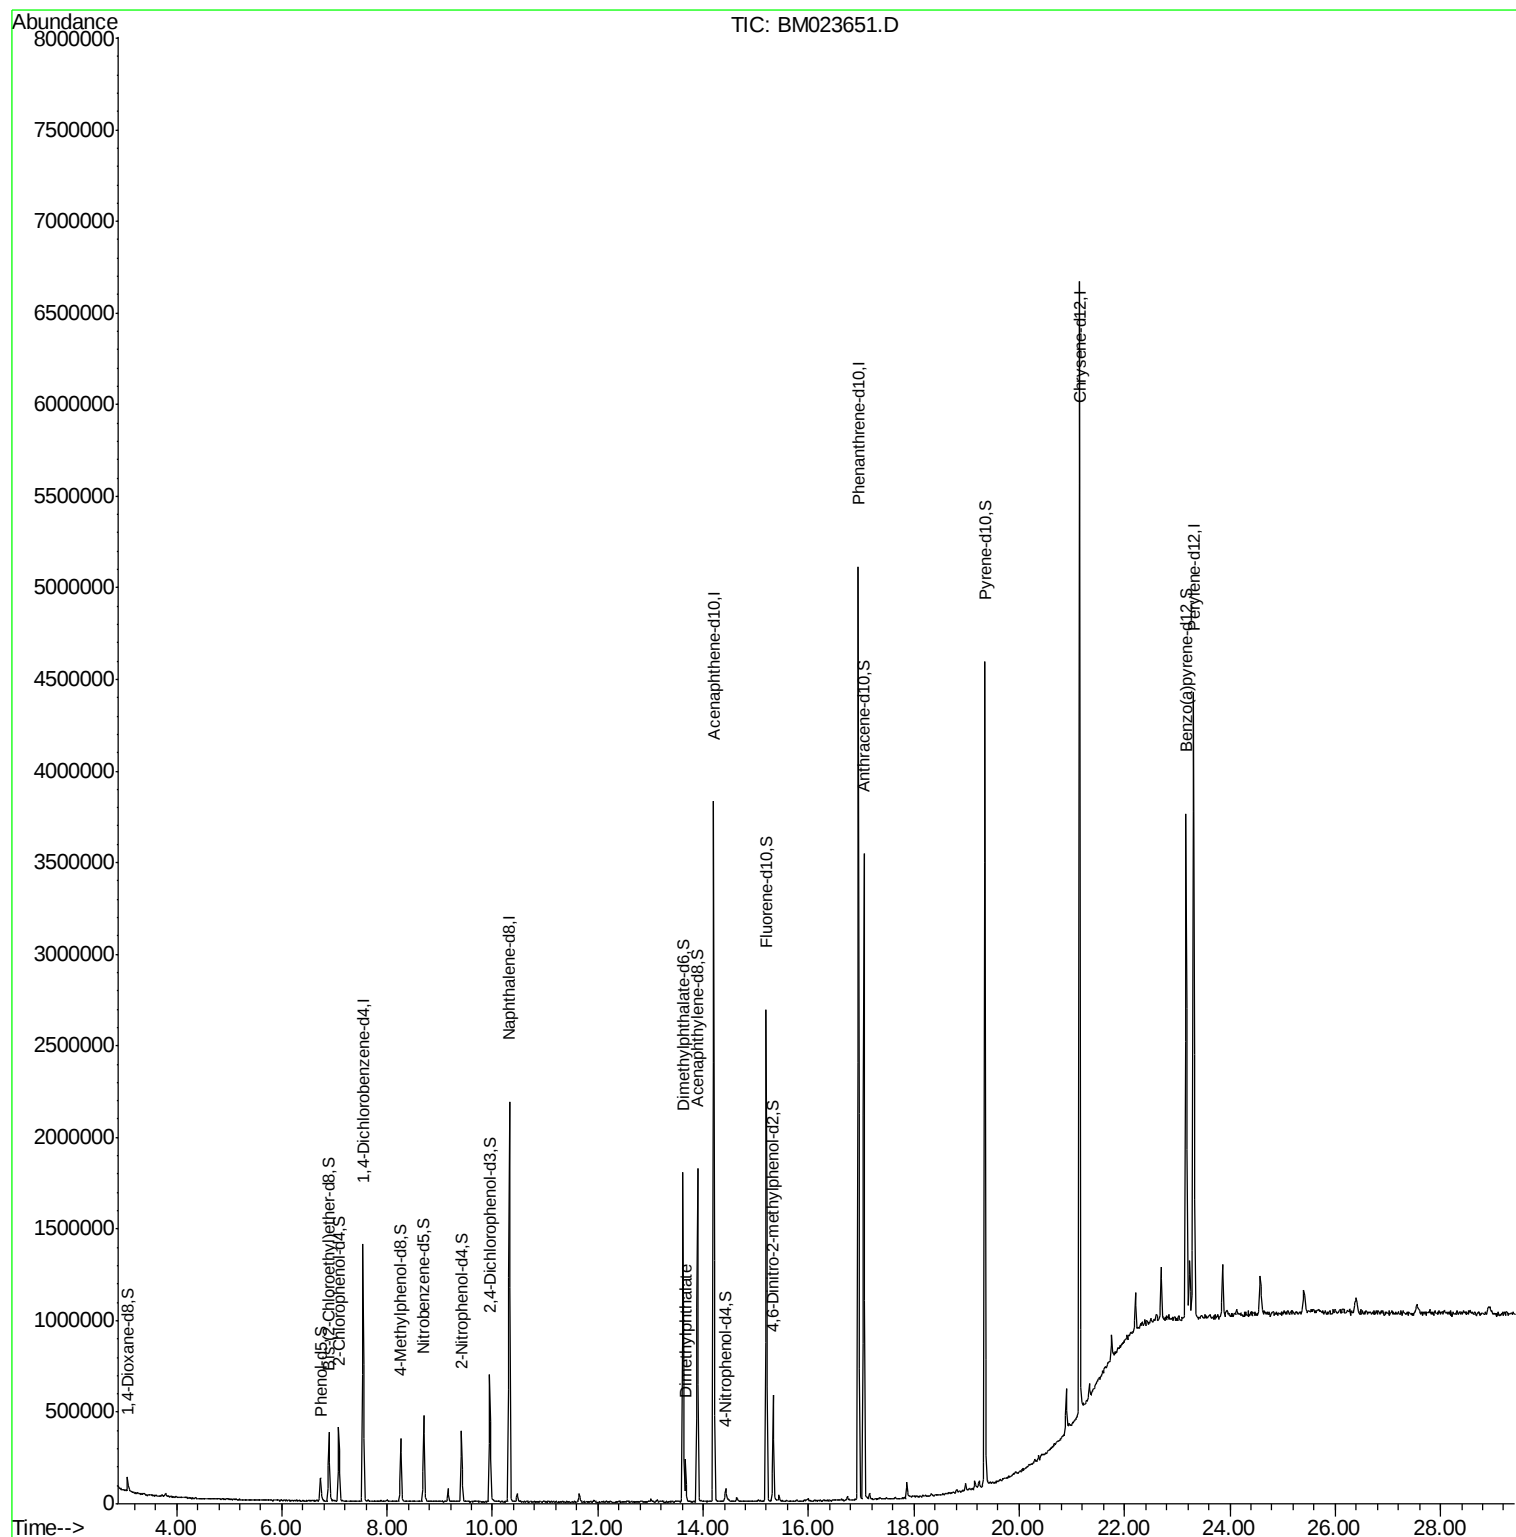

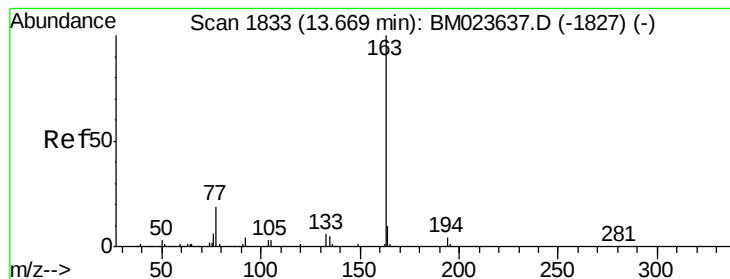

#45

Dimethylphthalate

Concen: 1.436 ng/ul

RT: 13.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: BM023651.D

Acq: 11 Nov 2019 23:52

Instrument :

BNA_M

ClientSampleId :

C0CQ1


Tot Ion:163 Resp: 141444

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2

164 11.1 8.0 12.0

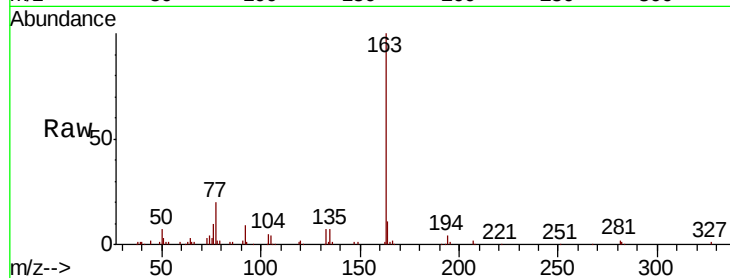

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

