

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111318\
 Data File : BM017631.D
 Acq On : 13 Nov 2018 21:25
 Operator : MJ/SJ
 Sample : J5916-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 110918-DBRI-F-U-S

Quant Time: Nov 14 03:34:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 12 18:37:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	212130	20.00	ng	0.00
21) Naphthalene-d8	10.39	136	862073	20.00	ng	0.00
39) Acenaphthene-d10	14.26	164	507316	20.00	ng	0.00
64) Phenanthrene-d10	17.02	188	1185786	20.00	ng	0.00
76) Chrysene-d12	21.22	240	1160905	20.00	ng	0.00
87) Perylene-d12	23.41	264	992504	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.24	112	561817	44.70	ng	0.00
7) Phenol-d6	6.80	99	429114	24.44	ng	0.00
23) Nitrobenzene-d5	8.77	82	1896467	113.57	ng	0.00
42) 2,4,6-Tribromophenol	15.76	330	758775	104.09	ng	0.00
45) 2-Fluorobiphenyl	12.87	172	4220722	107.93	ng	0.00
79) Terphenyl-d14	19.66	244	5849456	114.20	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.74	163	90309	2.189	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111318\
Data File : BM017631.D
Acq On : 13 Nov 2018 21:25
Operator : MJ/SJ
Sample : J5916-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
110918-DBRI-F-U-S

Quant Time: Nov 14 03:34:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

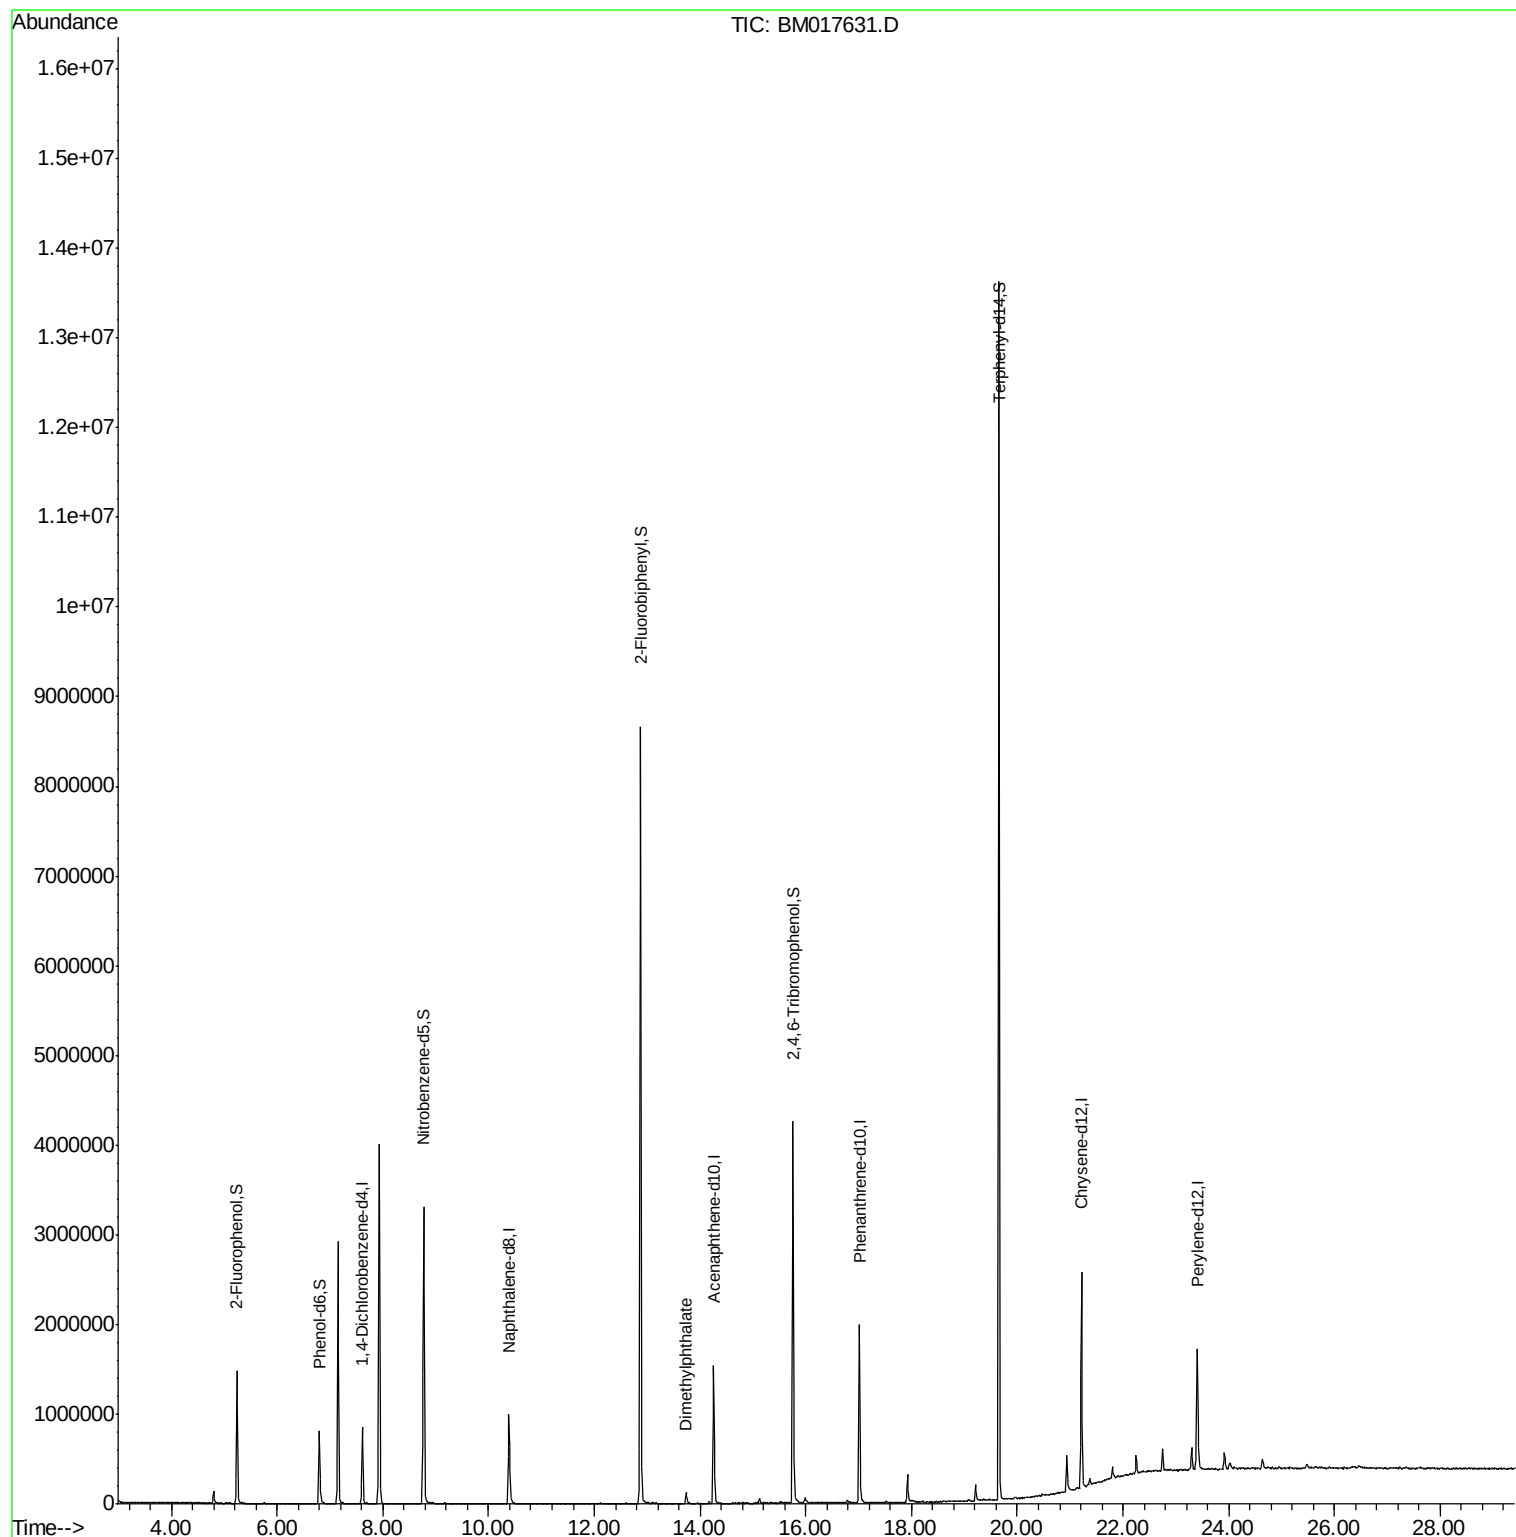

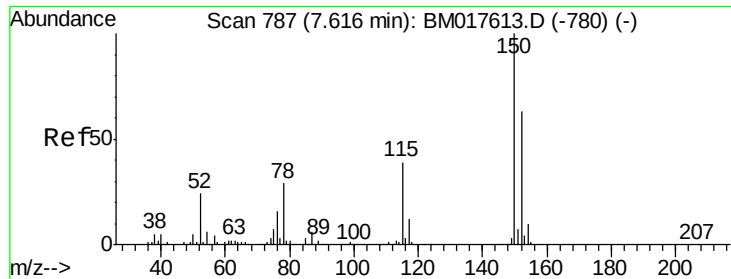


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.62 min Scan# 787
Delta R.T. 0.00 min
Lab File: BM017631.D
Acq: 13 Nov 2018 21:25

Instrument :
BNA_M
ClientSampleId :
110918-DBRI-F-U-S

Tgt Ion	Ratio	Lower	Upper
152	100		
150	154.7	126.4	189.6
115	59.7	49.4	74.0



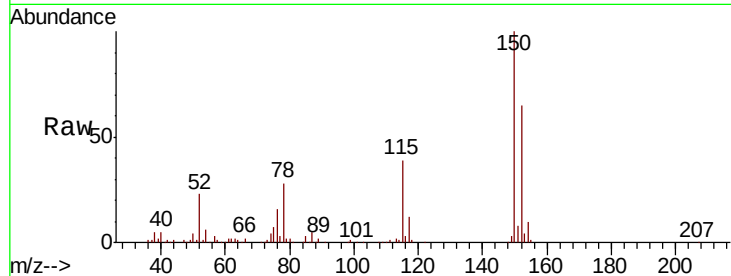


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

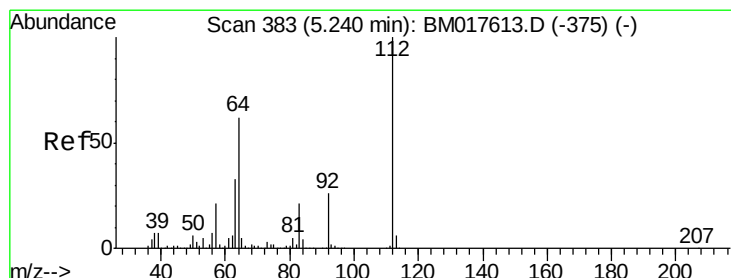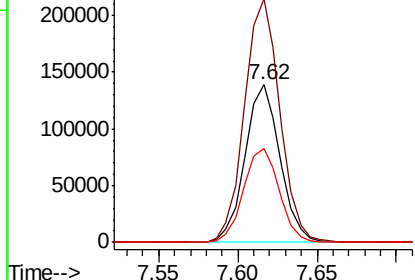

#5

2-Fluorophenol
Concen: 44.697 ng
RT: 5.24 min Scan# 383
Delta R.T. 0.00 min
Lab File: BM017631.D
Acq: 13 Nov 2018 21:25

Tgt Ion	Ratio	Lower	Upper
112	100		
64	62.3	49.3	73.9
63	33.9	26.2	39.4


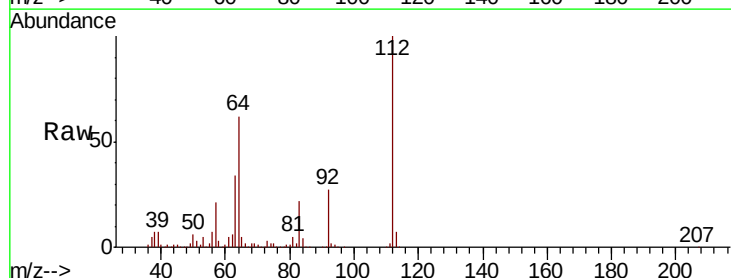



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

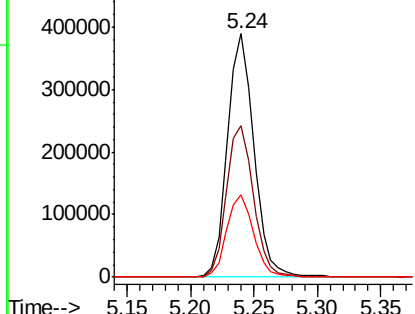



#7

Phenol-d6

Concen: 24.444 ng

RT: 6.80 min Scan# 648

Delta R.T. -0.01 min

Lab File: BM017631.D

Acq: 13 Nov 2018 21:25

Instrument :

BNA_M

ClientSampleId :

110918-DBRI-F-U-S


Tgt Ion: 99 Resp: 429114

Ion Ratio Lower Upper

99 100

42 21.9 16.3 24.5




71 38.1 29.8 44.8

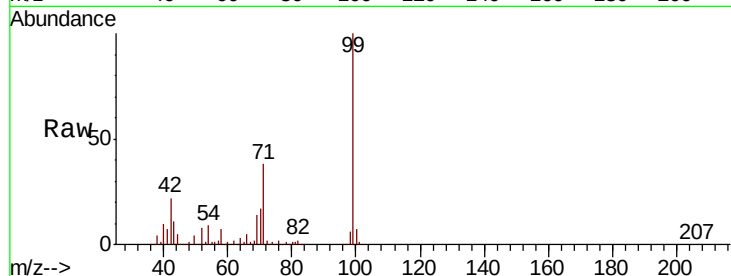

Abundance Ion 99.00 (98.70 to 99.70): BM017613.D (-641) (-)

Ion 42.00 (41.70 to 42.70): BM017613.D (-641) (-)

Ion 71.00 (70.70 to 71.70): BM017613.D (-641) (-)

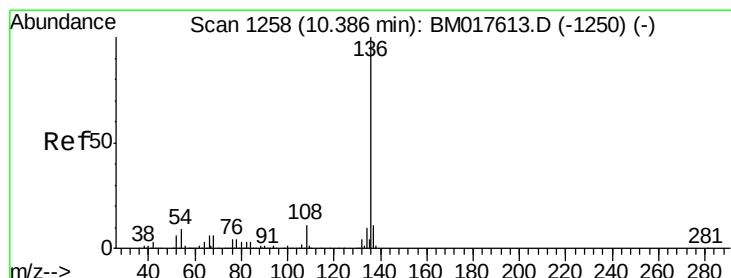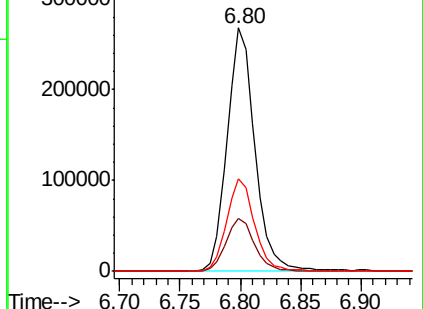

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.39 min Scan# 1258

Delta R.T. 0.00 min

Lab File: BM017631.D

Acq: 13 Nov 2018 21:25

Tgt Ion: 136 Resp: 862073


Ion Ratio Lower Upper

136 100

137 10.6 8.6 12.8

54 9.1 7.0 10.6

68 5.6 4.9 7.3


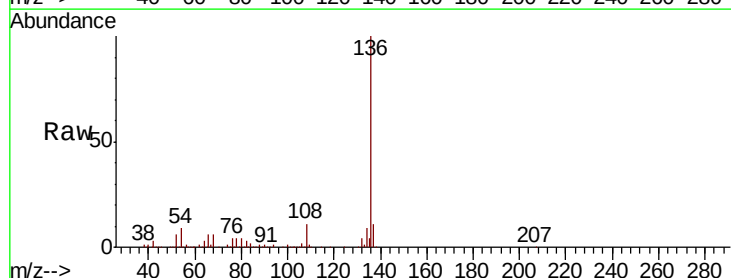



Abundance Ion 136.00 (135.70 to 136.70): BM017613.D (-1250) (-)

Ion 137.00 (136.70 to 137.70): BM017613.D (-1250) (-)

Ion 54.00 (53.70 to 54.70): BM017613.D (-1250) (-)

Ion 68.00 (67.70 to 68.70): BM017613.D (-1250) (-)

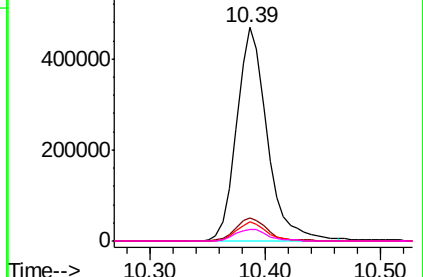







#23
Nitrobenzene-d5
Concen: 113.570 ng
RT: 8.77 min Scan# 984
Delta R.T. 0.00 min
Lab File: BM017631.D
Acq: 13 Nov 2018 21:25

Instrument :
BNA_M
ClientSampleId :
110918-DBRI-F-U-S

Tgt Ion: 82 Resp: 1896467
Ion Ratio Lower Upper
82 100
128 41.6 33.0 49.4
54 52.5 41.4 62.2

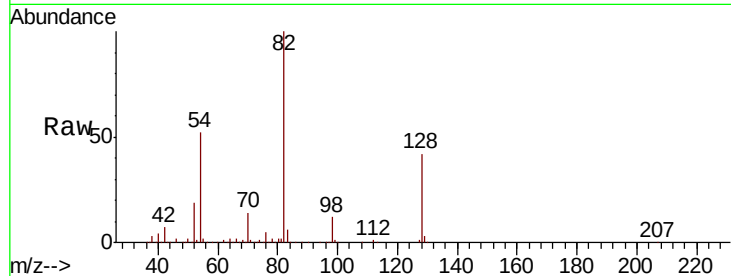


Abundance Ion 82.00 (81.70 to 82.70): BM017631.D (-967) (-)
Ion 128.00 (127.70 to 128.70): BM017631.D (-967) (-)
Ion 54.00 (53.70 to 54.70): BM017631.D (-967) (-)

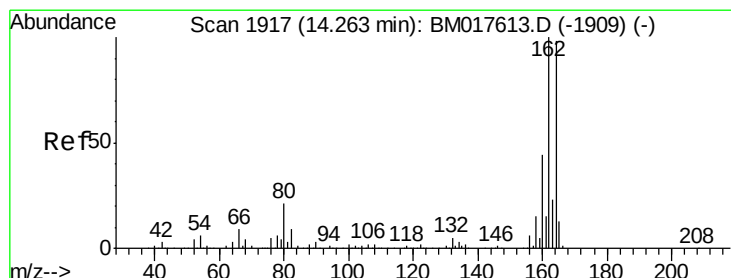
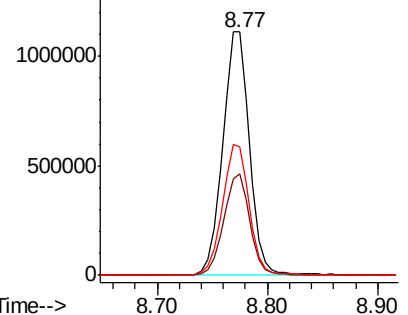



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.26 min Scan# 1917
Delta R.T. 0.00 min
Lab File: BM017631.D
Acq: 13 Nov 2018 21:25

Tgt Ion: 164 Resp: 507316
Ion Ratio Lower Upper
164 100
162 103.4 81.4 122.0
160 44.9 35.6 53.4

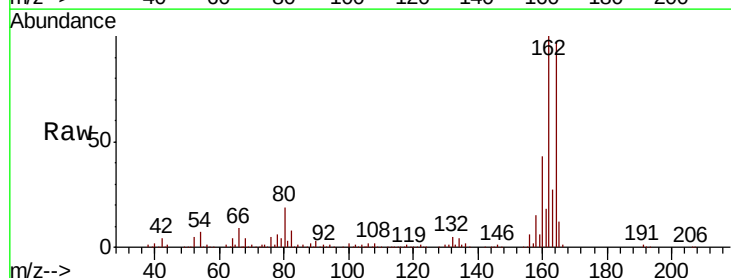

Abundance Ion 164.00 (163.70 to 164.70): BM017631.D (-1900) (-)
Ion 162.00 (161.70 to 162.70): BM017631.D (-1900) (-)
Ion 160.00 (159.70 to 160.70): BM017631.D (-1900) (-)

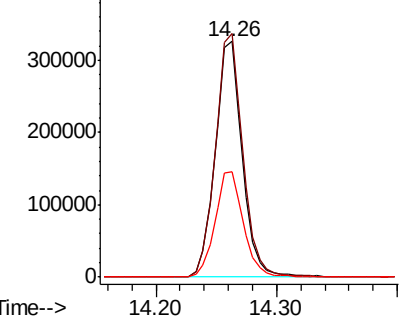


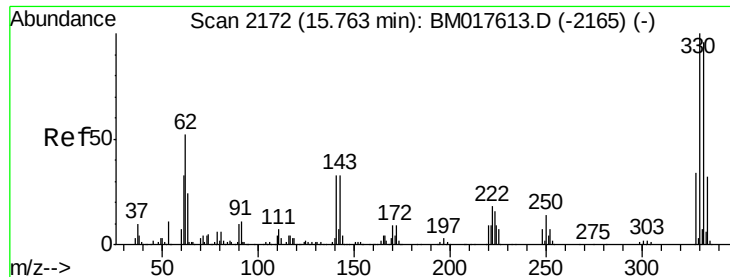




#42
 2,4,6-Tribromophenol
 Concen: 104.093 ng
 RT: 15.76 min Scan# 2172
 Delta R.T. 0.00 min
 Lab File: BM017631.D
 Acq: 13 Nov 2018 21:25

Instrument :
 BNA_M
 ClientSampleId :
 110918-DBRI-F-U-S

Tgt Ion:330 Resp: 758775
 Ion Ratio Lower Upper
 330 100
 332 97.1 77.9 116.9
 141 37.9 27.5 41.3

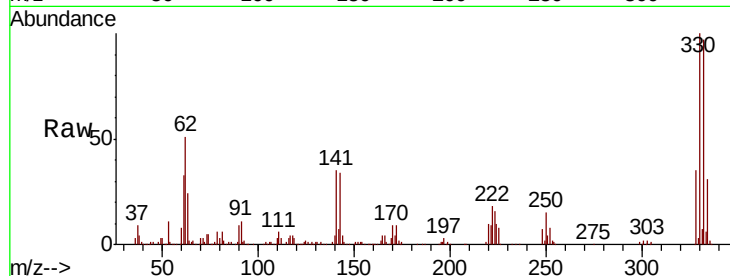


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

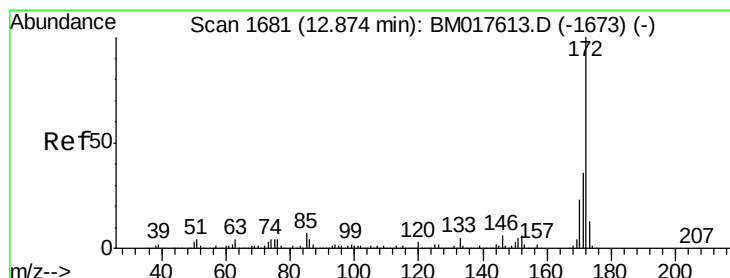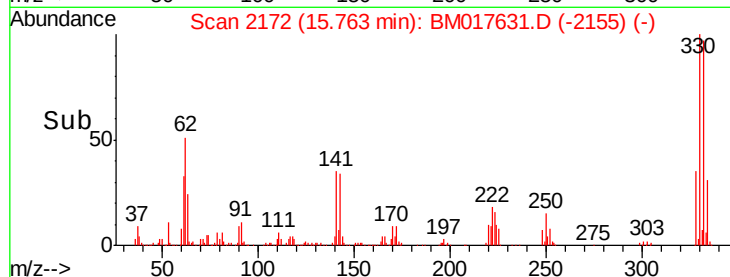
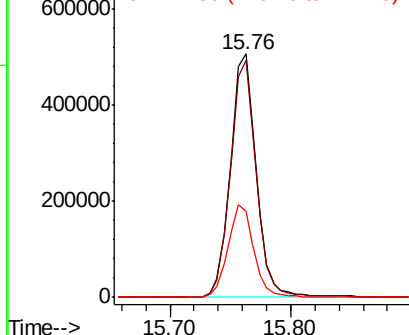



#45
 2-Fluorobiphenyl
 Concen: 107.934 ng
 RT: 12.87 min Scan# 1681
 Delta R.T. 0.00 min
 Lab File: BM017631.D
 Acq: 13 Nov 2018 21:25

Tgt Ion:172 Resp: 4220722
 Ion Ratio Lower Upper
 172 100
 171 35.2 28.7 43.1
 170 22.9 18.3 27.5

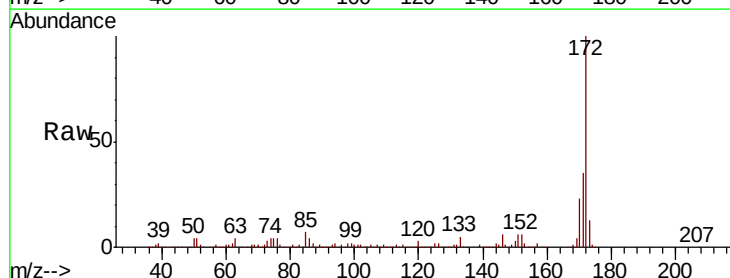

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

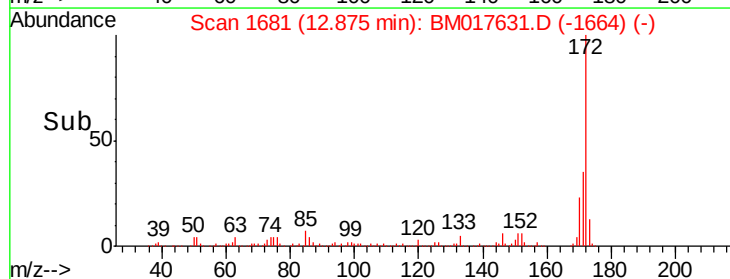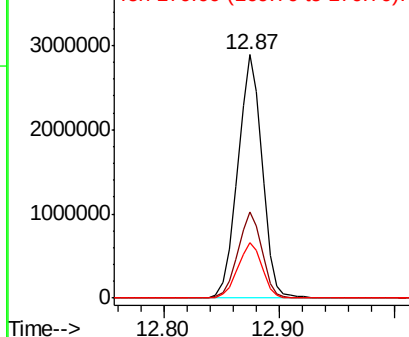

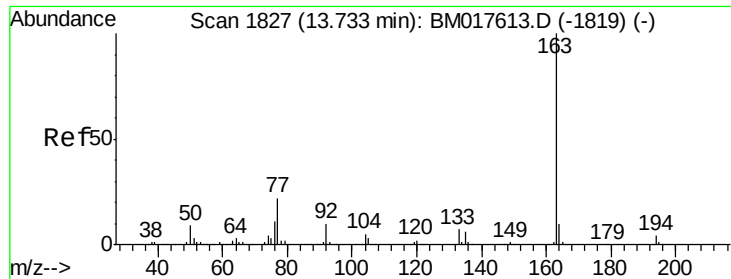

#50

Dimethylphthalate

Concen: 2.189 ng

RT: 13.74 min Scan# 1828

Delta R.T. 0.01 min

Lab File: BM017631.D

Acq: 13 Nov 2018 21:25

Instrument :

BNA_M

ClientSampleId :

110918-DBRI-F-U-S


Tgt Ion:163 Resp: 90309

Ion Ratio Lower Upper

163 100

194 4.2 3.1 4.7




164 10.3 8.2 12.4

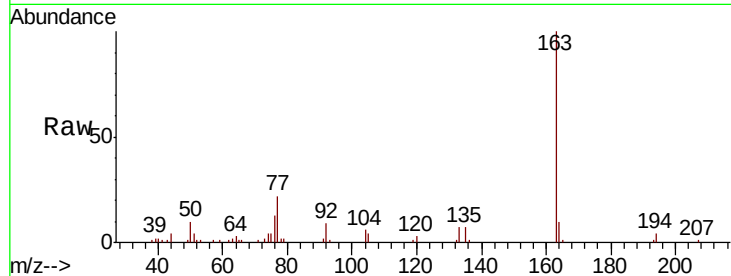

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

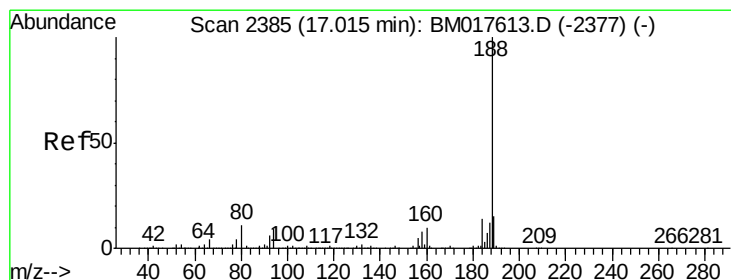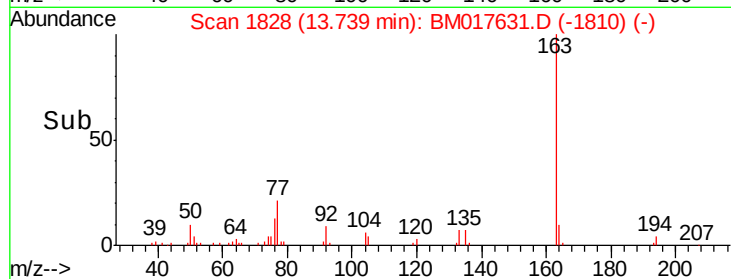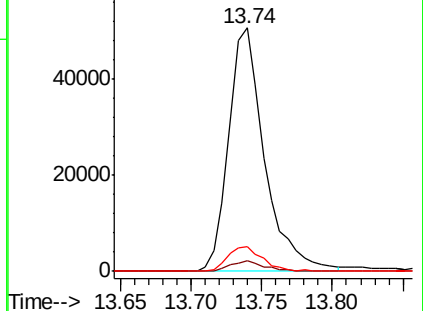

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.02 min Scan# 2385

Delta R.T. 0.00 min

Lab File: BM017631.D

Acq: 13 Nov 2018 21:25


Tgt Ion:188 Resp: 1185786

Ion Ratio Lower Upper

188 100

94 8.5 7.5 11.3



80 10.1 8.6 13.0

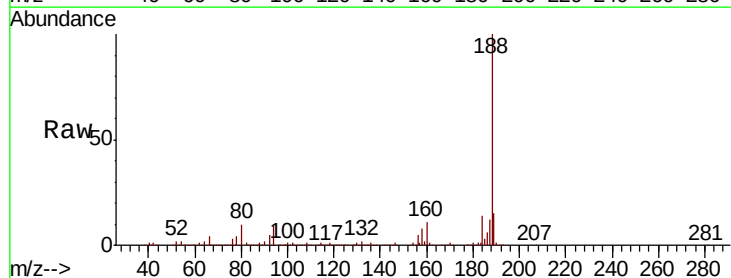


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

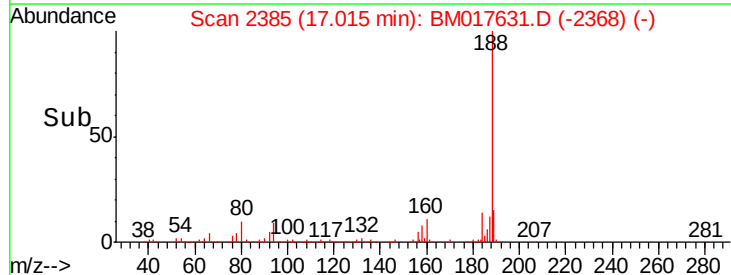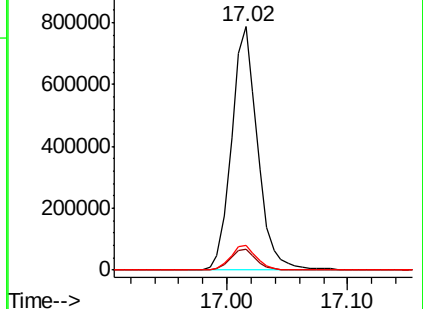

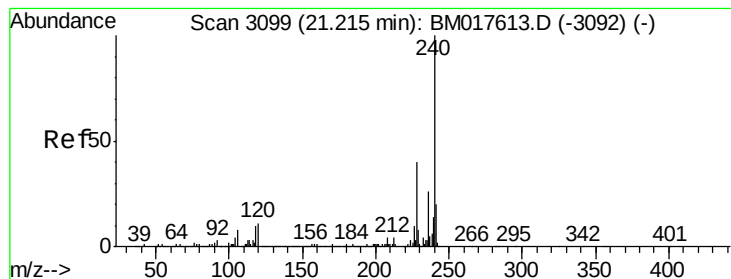

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.22 min Scan# 3099

Delta R.T. 0.00 min

Lab File: BM017631.D

Acq: 13 Nov 2018 21:25

Instrument :

BNA_M

ClientSampleId :

110918-DBRI-F-U-S


Tgt Ion:240 Resp: 1160905

Ion Ratio Lower Upper

240 100

120 9.3 8.5 12.7

236 25.1 20.4 30.6



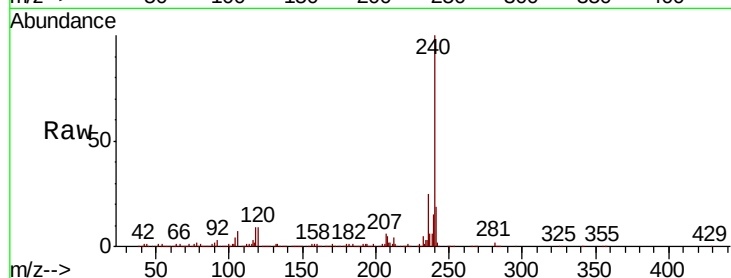


Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

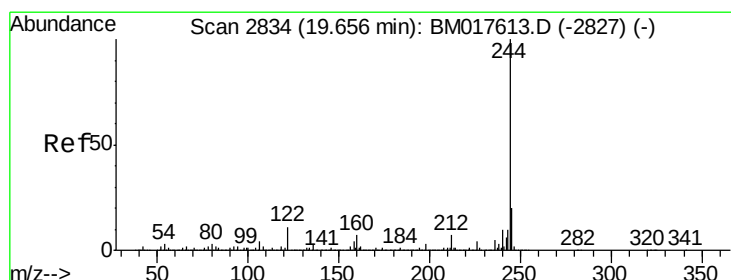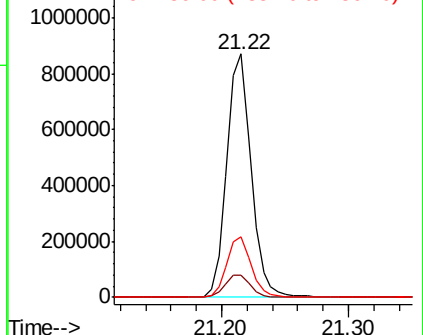

#79

Terphenyl-d14

Concen: 114.198 ng

RT: 19.66 min Scan# 2834

Delta R.T. 0.00 min

Lab File: BM017631.D

Acq: 13 Nov 2018 21:25


Tgt Ion:244 Resp: 5849456

Ion Ratio Lower Upper

244 100

212 7.6 5.8 8.6

122 11.2 9.0 13.6


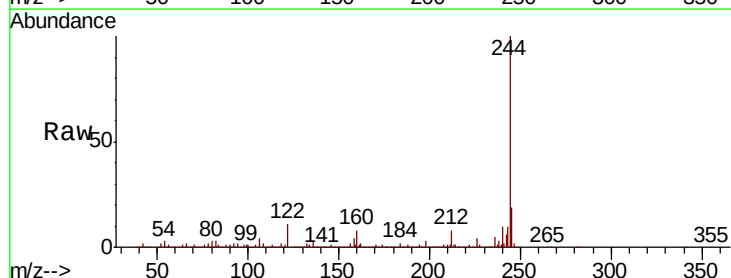



Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

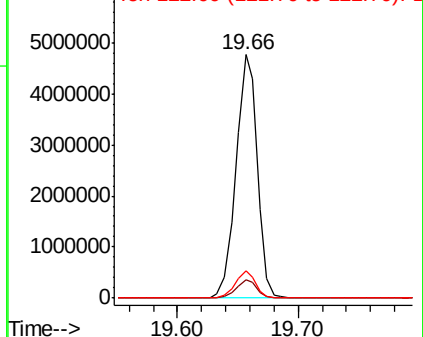

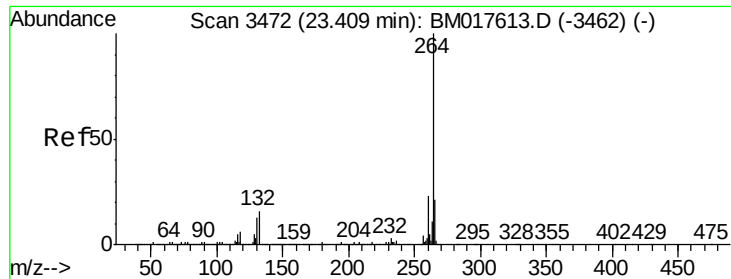

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.41 min Scan# 3472
Delta R.T. 0.00 min
Lab File: BM017631.D
Acq: 13 Nov 2018 21:25

Instrument :
BNA_M
ClientSampleId :
110918-DBRI-F-U-S

Tgt Ion:	264	Resp:	992504
Ion	Ratio	Lower	Upper
264	100		
260	23.6	18.2	27.2
265	22.2	17.5	26.3

